

CochlearTM Nucleus[®] CI632 cochlear implant with Slim Modiolar electrode

Physician's Guide

Asia Pacific



Hear now. And always

About this guide

This guide applies to the Cochlear™ Nucleus® CI632 cochlear implant, which is a CI600 Series implant.

This guide is intended for surgical staff involved in implanting the device.

Surgeons implanting the device should be experienced in cochlear implant surgery.

Before surgery, ensure you are thoroughly familiar with the information in this guide and the product labelling. The guide includes important information on MRI, indications, contraindications, adverse effects, warnings and precautions. A surgical procedure for implanting the device is also explained.

This guide does not take account of any particular circumstances or factors relevant to an individual patient or case. Other surgical approaches and variations are practised and may be more appropriate in certain circumstances. After considering all relevant circumstances, factors and information in each case, the appropriate surgical procedure is determined by the relevant physician exercising independent medical judgment.

Symbols used in this guide



Note

Important information or advice.



Caution (no harm)

Special care to be taken to ensure safety and effectiveness.
Could cause damage to equipment.



Warning (harmful)

Potential safety hazards and serious adverse reactions.
Could cause harm to person.

Contents

About this guide.....	1
Symbols used in this guide	2
Warnings and Cautions for device use	6
Warnings.....	6
Cautions.....	8
Note.....	8
Intended use and indications	9
Intended use	9
Indications.....	9
Benefits.....	11
Bilateral hearing loss	11
Unilateral hearing loss	12
Children.....	12
All implant recipients.....	12
Contraindications	13
Adverse effects.....	14
Meningitis.....	15
Loss of residual hearing.....	15
Device description	16
Implanted component.....	16
External components.....	16
New features.....	17
The CI632 cochlear implant with Slim Modiolar electrode.....	18
Surgical instruments and accessories.....	20
Reusable after reprocessing.....	22
Single-use sterile.....	24
Non-sterile	28

Surgical procedure.....	29
Pre-incision: non-sterile field	30
Opening the CI500 Series Sterile Silicone Implant Template	31
Incision and periosteal pocket	32
Mastoidectomy and preparing the bone recess.....	33
Drilling tie-down holes.....	36
Opening the facial recess (Posterior Tympanotomy).....	37
Preparing the round window or cochleostomy	38
Inspecting the implant, electrodes and sizing tool.....	42
Positioning and securing the implant	43
Securing the extracochlear electrode	44
Inserting the intracochlear electrode	45
Securing and sealing the intracochlear electrode.....	55
Performing intraoperative measurements	57
Closure	58
Post-operative management.....	59
Fitting the sound processor.....	59
Registering the implant	59
Identifying the implant.....	60
Explanting the implant	60
Reporting problems.....	61
MRI safety information.....	62
Removing the magnet cassette	63
Replacement magnet cassettes and non-magnetic cassettes	64
Removing the magnet cassette before implantation.....	65
Removing and replacing the magnet cassette or non-magnetic cassette after implantation	70

How the implant is supplied	75
Transport and handling	75
Storage	75
CI632 implant specifications.....	76
General information.....	79
Warranty.....	79
Symbols	79
Privacy and the collection of personal information	81

Warnings and Cautions for device use

This section does not contain all the important information required to use and implant the device, only critical information to implant the device safely and effectively. Read the full *Physician's Guide* before implanting the device.

Warnings

Pre-operative

- **Meningitis** is a known risk of inner ear surgery. You should counsel candidates of this risk and determine their immunisation status for micro-organisms that cause meningitis.
- **Wound infection** after cochlear implant surgery or explantation may be prevented by administering broad-spectrum antibiotic before and during surgery.
- The implant is sterilised using **ethylene oxide (EtO)**. After the sterilisation process, residual EtO is less than 0.4 mg per device. This residual level is suitable for a recipient with a body weight of 7 kg or greater.*

* Calculated with guidance from EN ISO 10993-7.

Medical treatments generating induced currents, heat and vibration

- **Electrosurgical instruments** can induce radio frequency currents that could flow through the electrode.

When using bipolar electrosurgical instruments on the head and neck of a patient, the cautery electrodes must not contact the implant and should be kept more than 1 cm (½ in) from the electrodes.

- **High currents** induced into the electrode lead can cause damage to cochlea and neural tissues, and the implant.

Do not use:

- **monopolar electrosurgical instruments** on the head or neck of an implant patient.
- **therapeutic or medical diathermy** (thermopenetration) using electromagnetic radiation (magnetic induction coils or microwave).
- **neurostimulation** directly over the implant.
- **Ultrasound fields** can be inadvertently concentrated at the implant and cause tissue damage or damage to the implant.

Do not use:

- **therapeutic levels of ultrasound energy** directly over the implant
- **medical diathermy using ultrasound** on the head and neck of an implant patient.
- **Electroconvulsive therapy** can cause tissue damage or damage to the implant. Do not use electroconvulsive therapy on an implant patient under any circumstances.

Magnetic Resonance Imaging (MRI)



The Cochlear Nucleus CI632 implant is **MR Conditional**. MRI is contraindicated except under specific circumstances. See *MRI safety information* on page 62.

Cautions

- When using **sharp instruments** near the implant, take care to avoid nicking or damaging the case, insulation, electrode lead, exposed magnet cassette cover or non-magnetic cassette cover.
- **Ionising radiation therapy** can cause damage to the implant. Do not use ionising radiation therapy directly over the implant.



Note

- **Facial nerve monitor** use is advised, particularly for cases where the facial nerve may be at greater risk such as congenital temporal bone anomalies and revision surgeries.

Intended use and indications

Intended use

Cochlear Nucleus CI600 Series implants are single use devices intended for long term implantation under the skin in the mastoid region of either side of the head. They are for professional use only.

Indications

A cochlear implant provides auditory sensation and sound perception by electrically stimulating the auditory nerve of a hearing-impaired ear.

The degree of hearing loss and compromised hearing with hearing aids must be established and verified clinically using age-appropriate measures before recommending unilateral or bilateral cochlear implants.

Prospective implant recipients and their families should be well motivated, willing to undergo hearing rehabilitation as needed and have appropriate expectations of the potential benefits of unilateral or bilateral implants.

A Cochlear Nucleus cochlear implant is intended for the following recipient groups.

Group A

Individuals aged up to 17 years who have clinically established bilateral or unilateral sensorineural hearing loss and who have compromised functional hearing with hearing aids or would receive no benefit with hearing aids. Typical preoperative threshold levels in the impaired ears demonstrate a pure-tone average loss of moderately severe to profound degree.*†

Group B

Individuals aged 18 years and older who have clinically established postlinguistic bilateral or unilateral sensorineural hearing loss and who have compromised functional hearing with hearing aids, or would receive no benefit with hearing aids. Typical preoperative threshold levels in the impaired ears demonstrate a pure-tone average loss of moderately severe to profound degree.*†

Group C

Prelinguistically or perilinguistically deafened individuals aged 18 years and older who have profound bilateral sensorineural hearing loss and who have compromised hearing with hearing aids.

* Pure-tone average loss can be defined as the average threshold calculated for four frequencies at 500, 1000, 2000 and 3000 or 4000 Hz as available. Reference: American Speech-Language-Hearing Association. (1981). *On the Definition of Hearing Handicap* [Relevant Paper]. Available from www.asha.org/policy.

† ANSI standards for defining hearing impairment quoted by ASHA. Available from www.asha.org/public/hearing/Degree-of-Hearing-Loss (Feb 2012).

Benefits

Bilateral hearing loss

Group A, B or C

Cochlear Nucleus cochlear implant recipients from group A, B or C with bilateral hearing loss will experience:

- detection of medium to loud environmental sounds at comfortable listening levels
- detection of conversational speech at comfortable listening levels.

Group A or B

Most Cochlear Nucleus cochlear implant recipients from group A or B with bilateral hearing loss will experience:

- improvement in speech recognition and communication ability with lip reading
- improvement in speech recognition without lip reading

Some Cochlear Nucleus cochlear implant recipients from group A or B with bilateral hearing loss will experience:

- limited improvement in the recognition of environmental sounds
- limited ability to use the telephone.

Unilateral hearing loss

Group A or B

Cochlear Nucleus cochlear implant recipients from group A or B with unilateral hearing loss will experience no change to the hearing status of the non-implanted ear.

Most Cochlear Nucleus cochlear implant recipients from group A or B with unilateral hearing loss will experience:

- improved identification of environmental sounds in the implanted ear
- improved speech recognition in a quiet environment in the implanted ear.

Some Cochlear Nucleus cochlear implant recipients from group A or B with unilateral hearing loss will experience:

- improvement in identifying the direction of environmental sounds and speech
- improvement in speech recognition in a noisy environment
- improvement in overall sound quality
- reduced tinnitus
- reduced fatigue when listening.

Children

Generally, children require considerably more listening experience, therapeutic and educational support than adults to achieve the benefits described above with their cochlear implants.

All implant recipients

In cases where the intracochlear array is partially inserted into the cochlea, recipients may not experience some of the benefits described above.

Contraindications

A Cochlear Nucleus cochlear implant is not suitable for individuals with the following conditions:

- deafness due to lesions of the acoustic nerve or central auditory pathway
- active middle ear infections
- absence of cochlear development
- tympanic membrane perforation in the presence of active middle ear disease
- ossification of the cochlea that prevents electrode insertion.

Adverse effects

Prospective Cochlear Nucleus cochlear implant recipients should be advised of the following possible effects of receiving an implant:

- Normal risks associated with surgery and general anaesthesia.
- Increased surgical and anaesthetic risks for certain populations.
- Complications most frequently associated with this surgical procedure—stimulation of the facial nerve, taste disturbance and tinnitus.
- Complications that may require additional medical treatment, surgery and/or removal of the device, such as:
 - Acute Otitis Media (AOM)
 - facial nerve injury leading to temporary facial nerve weakness
 - perilymph fistula
 - Concurrent Cerebrospinal Fluid (CSF) leakage
 - vestibular dysfunction
 - subdural injury
 - subcutaneous haematoma
 - irritation, inflammation or breakdown of the skin flap; infection; and in some cases, extrusion of the device caused by the presence of a foreign body under the skin
 - decreased hearing ability caused by the electrode array migrating partially or completely out of the cochlea
 - perforation of external ear structures, such as the tympanic membrane or canal wall, by the electrode lead
 - perception of non-auditory sensations and poorer performance than expected from misplacement of the electrode array.

- Electrical stimulation may result in increased tinnitus, temporary facial nerve stimulation, temporary dizziness, or temporary pain.
- The long term effects of electrode insertion trauma or chronic electrical stimulation are unknown. Such effects may include new bone growth in the cochlea or deterioration of the nerve cells. These effects may preclude replacement of the electrode array or may lead to eventual deterioration of cochlear response.
- Failure of component parts (both external and internal) could result in the perception of an uncomfortably loud sound sensation, intermittent sound, or no sound.
- Failure of various component parts of the implanted device could require removal or replacement of the implant, or a reduction in the number of electrodes used.

Meningitis

Before implantation, candidates should consult their primary care physician and implanting surgeon regarding vaccination status against micro-organisms that cause meningitis.

Meningitis is a known risk of inner ear surgery and candidates should be appropriately counselled of this risk. Certain preoperative conditions may increase the risk of meningitis with or without an implant. These conditions include:

- Mondini's syndrome and other congenital cochlear malformations
- CSF shunts or drains
- recurrent episodes of bacterial meningitis before implantation
- perilymph fistulas and skull fracture/defect with CSF communication.

Loss of residual hearing

Inserting the electrode into the cochlea may result in complete loss of residual hearing in the implanted ear.

Device description

Cochlear Nucleus cochlear implant systems are designed to provide useful hearing. The system works by converting sound in the environment into electric pulses that stimulate the auditory nerve, allowing the brain to perceive sound.

The Cochlear Nucleus cochlear implant system has implanted and external components.

Implanted component

The cochlear implant is surgically implanted under the skin behind the ear. It includes a receiver/stimulator to receive and decode the electrical signals from the sound processor and an electrode to deliver these signals to the cochlea.

External components

The external components include a sound processor, and associated accessories and cables.

The system is programmed by a Cochlear proprietary programming system.

For information on compatibility between implants and processors, refer to the *Custom Sound® User Guide*.

New features

CI600 Series implants have implant coil plates either side of a magnet pocket which contains a removable magnet cassette. This design allows for magnet removal and replacement from the distal end of the implant coil, if required.



Figure 1: CI632 cochlear implant with magnet cassette partially removed from pocket

The CI632 cochlear implant with Slim Modiolar electrode

The CI632 implant is a CI600 Series implant.

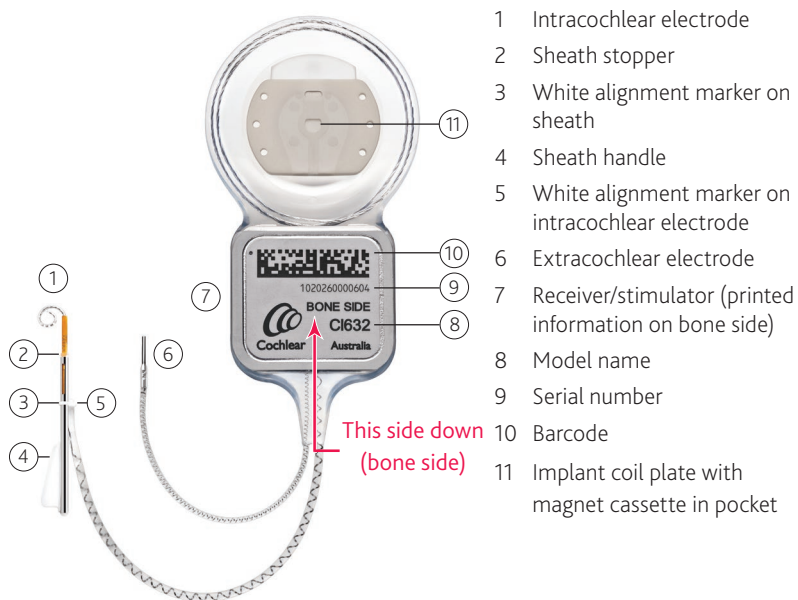


Figure 2: CI632 cochlear implant with Slim Modiolar electrode (bone side)

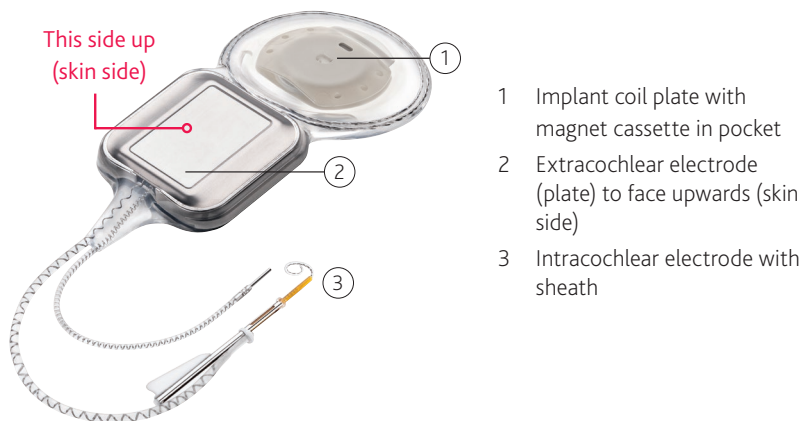


Figure 3: CI632 cochlear implant with Slim Modiolar electrode (skin side)

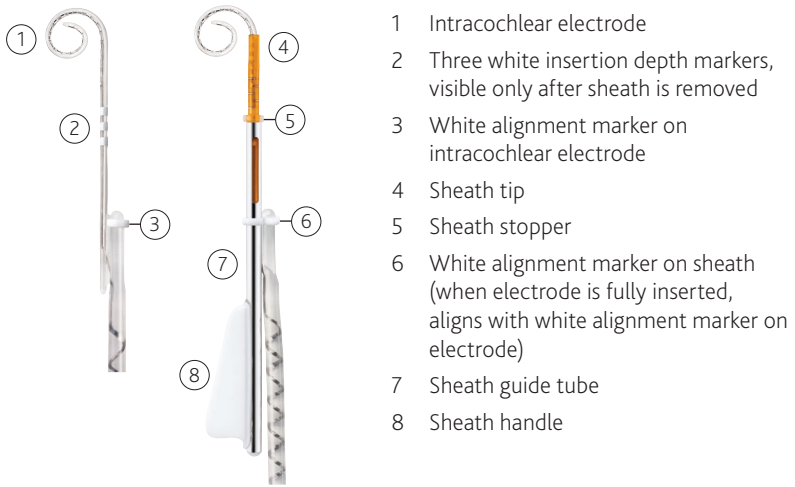


Figure 4: Slim Modiolar electrode with sheath removed and with sheath

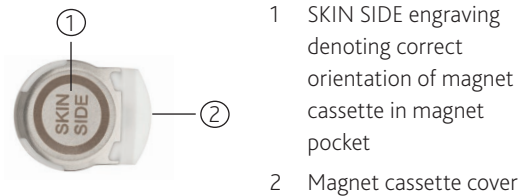


Figure 5: Cochlear Nucleus Magnet Cassette (skin side)

Surgical instruments and accessories

Instruments and accessories in this section are appropriate for use with Cochlear Nucleus CI600 Series implants.

All items except the Sterile Silicone Implant Template are available to be ordered individually. As indicated below, some items are included in the CI500 Series Surgical Instrument Kit. An upgrade kit is also available.

Instruments	Product code	CI500 Series Instrument Kit	CI500 Series Instrument Upgrade Kit
AOS™ Forceps for the Contour Advance® Electrode	Z60770	✓	✓
BTE Template	Z33011	✓	—
CI500 Series Recess Gauge	Z139274	✓	✓
CI500 Series Implant Template	Z139273	✓	✓
Contour® Electrode Claw	Z33021	✓	—
Electrode Claw (Straight)	Z30090	—	—
Contour Advance® Depth Gauge	Z179994	—	—
Depth Gauge (Straight)	Z60006	—	—
CI500 Series Sterile Silicone Implant Template*	S211296	—	—
CI500 Series Non-Sterile Silicone Implant Template	Z179609	—	—
Spacer for Intraoperative Testing	Z33012	—	—
Cochleostomy Sizing Tool*	S407840	—	—
Accessories			
Non-Magnetic Cassette	P782484	—	—
Replacement Magnet Cassette	P782485	—	—

* Supplied with implant; not available separately

Items used with the Cochlear Nucleus CI632 cochlear implant are referenced in the *Surgical procedure* and *MRI safety information* sections of this guide.

Dispose of used items according to your institution's policy on the disposal of used instruments and accessories.



Warning

Do not use surgical instruments or accessories supplied or intended to be sterile if they become non-sterile, e.g. if dropped or mishandled in theatre.

Reusable after reprocessing

These instruments are stainless steel, and can be cleaned and resterilised as instructed in the *Surgical Instrument Sterilisation Reprocessing Guide*.

AOS™ Forceps for the Contour Advance® Electrode

Z60770



Used to grasp or hold the Contour Advance electrode during its insertion into the cochlea. Curved tip ends gently cup the array to improve stability and minimise rotation.



Caution

To avoid damaging the electrode, before each use hold forceps tips closed and ensure they are parallel and aligned. If not, do not use, as it may be difficult to release the electrode after insertion.

BTE Template

Z33011



Used to ensure the implant position provides space for a behind-the-ear sound processor.

CI500 Series Recess Gauge

Z139274



Used to mark the bone recess on the skull, measure the depth of the bone recess and check the location of the electrode exit excavation after drilling.

CI500 Series Implant Template

Z139273



Used to determine, or check, the shape of the implant bone recess excavation and the position of the implant.

Contour Electrode Claw

Z33021



Aids insertion of the Contour Advance electrode into the cochlea.
Gold-plated handle.

Electrode Claw (Straight)

Z30090



Aids insertion of the Straight electrode into the cochlea.



Single-use sterile

These items are supplied sterile for single-use only.



Warning

Do not resterilise. Do not use more than once. Re-use could cause infection.

Non-Magnetic Cassette		P782484
	If the recipient requires single or multiple MRI examinations on the head, a non-magnetic cassette is used to replace the magnet cassette.	
	For more information see <i>MRI safety information</i> on page 62.	
Replacement Magnet Cassette		P782485
	Used to replace a non-magnetic cassette after MRI examinations are complete.	
	For more information see <i>MRI safety information</i> on page 62.	



Note

- Non-magnetic cassettes and replacement magnet cassettes are supplied in a silicone carrier, as illustrated below. Remove the cassette from the silicone carrier before use.



- When marking the incision site, the silicone carrier can be used as a template. For details see *Removing and replacing the magnet cassette or non-magnetic cassette after implantation* on page 70.

Cochleostomy Sizing Tool

S407840



- 1 Stopper – 1.4 mm diameter
- 2 Tip – 0.8 mm diameter



Packed in the implant tray (white seal).

Used to determine/check the size of the cochleostomy or round window, to confirm if the electrode with sheath will fit.

Using the sizing tool to test the opening confirms if the sheath stopper will prevent the sheath and electrode from advancing too far into the cochlea.

Depth Gauges	
Contour Advance Depth Gauge Z179994	Depth Gauge (Straight) Z60006
	

Depth gauges are typically used in the sterile field when:

- pre-operative imaging to assess cochlea patency is inconclusive or unavailable, and
- it is suspected that cochlear obstruction such as ossification may prevent successful electrode insertion.

Use of depth gauges is not intended for normal cochleae where there is no suspicion of obstruction or malformation.

For more information refer to the appropriate *Depth Gauge User Guide*.

CI500 Series Sterile Silicone Implant Template

S211296

Used in the sterile field to check periosteal pocket size, implant bone recess shape and depth, and tie-down hole positions.

Provided with the implant; not available separately. For more information see warnings below and 2. *Opening the CI500 Series Sterile Silicone Implant Template* on page 31.

**Warning**

- For temporary use only. Not for implantation.
 - Supplied sterile. Sterilised in ethylene oxide. Do not resterilise.
 - Single-use item. Do not use more than once. Re-use could cause infection.
 - Do not use if packaging is damaged.
 - Do not use if item becomes non-sterile e.g. dropped or mishandled in theatre after removal from packaging.
 - Use with CI500 and CI600 Series implants only.
-

Non-sterile

These items are supplied non-sterile and are single use. They should not be sterilised.



Warning

Do not use more than once. Re-use could cause infection.

CI500 Series Non-Sterile Silicone Implant Template

Z179609

Used to determine/check the optimum implant position and mark it on the skin before incision.



Warning

Do not use in the sterile field. Use in the sterile field could cause infection.



Spacer for Intraoperative Testing

Z33012

When the processor coil is placed directly over the implant coil, use the spacer to ensure there is enough distance between the coils.



Warning

Must be used in a sterile sleeve. Use without a sterile sleeve could cause infection.



Surgical procedure

The surgical procedure described in this guide is only one approach to implanting the Cochlear Nucleus cochlear implant.

The surgical procedure includes the following:

1. Pre-incision: non-sterile field – page 30
2. Opening the CI500 Series Sterile Silicone Implant Template – page 31
3. Incision and periosteal pocket – page 32
4. Mastoidectomy and preparing the bone recess – page 33
5. Drilling tie-down holes – page 36
6. Opening the facial recess (Posterior Tympanotomy) – page 37
7. Preparing the round window or cochleostomy – page 38
8. Inspecting the implant, electrodes and sizing tool – page 42
9. Positioning and securing the implant – page 43
10. Securing the extracochlear electrode – page 44
11. Inserting the intracochlear electrode – page 45
12. Securing and sealing the intracochlear electrode – page 55
13. Performing intraoperative measurements – page 57
14. Closure – page 58

Where a surgical instrument is mentioned in the procedure, see *Surgical instruments and accessories* on page 20.

1. Pre-incision: non-sterile field

1. Place the BTE Template in position on the ear. Ensure there will be sufficient clearance between the receiver/stimulator and an ear level sound processor so that the sound processor will not rest on the receiver/stimulator.
2. Place the Non-sterile Silicone Implant Template on the skin so that the antero-inferior edge is at least 10 mm behind the edge of the BTE Template and above the canthomeatal line. Angle the Non-sterile Silicone Implant Template 30 to 45 degrees postero-superiorly, to lie on a flat portion of the skull. Mark its position on the scalp.



Note

For bilateral patients, position the second receiver/stimulator so that it is symmetrical with the first.

3. Mark the incision with a marking pen. Allow at least 15 mm between the implant and the incision.
The incision must be large enough to accommodate the cochlear implant. The flap may be inferiorly- or anteriorly-based but must allow the surgeon to secure the implant to the bone.
4. The Implant Template can be used to mark the position of the electrode lead exit for the proposed bone excavation for the receiver/stimulator. Mark with a drop of methylene blue on the bone using a 21 gauge needle through the skin.
5. Before incision, the incision line may be infiltrated with local anaesthetic and 1:100 000 or 1:200 000 adrenaline, or epinephrine, unless contraindicated.

2. Opening the CI500 Series Sterile Silicone Implant Template

One CI500 Series Sterile Silicone Implant Template is packaged with each implant. For warnings and more information see *CI500 Series Sterile Silicone Implant Template* on page 27.

To open the template tray:

Non-sterile field

1. Remove the cardboard box (outer packaging).
2. Break the seal on the outer tray, and confirm that:
 - exposure to ethylene oxide processing is indicated by a green dot on the outer tray
 - the two inner trays are not damaged.
3. Notice that the tray containing the Sterile Silicone Implant Template has a blue stripe. The tray containing the cochlear implant and sizing tool displays the Cochlear logo and has a white seal.



Warning

If the sterile pack is damaged do not use the template.

Sterile field

4. Remove the template tray (blue stripe) and break the seal.



Note

Keep the cochlear implant tray (white seal) to one side, within the sterile field, with the seal intact until later in the surgery.

5. Lift the Sterile Silicone Implant Template from the tray.

3. Incision and periosteal pocket



Warning

If the patient has an implant in the other ear, do not use monopolar electro-surgical instruments. Bipolar electro-surgical instruments may be used.

1. Make the incision down to the avascular plane of the periosteum and temporalis fascia, long enough to provide sufficient access. Stabilise the area using retraction as necessary.
2. Use the Implant Template or the Sterile Silicone Implant Template to check the position of the implant.
3. Incise the underlying periosteum and lower portion of the temporalis fascia creating a fibromuscular/periosteal flap based either anteriorly or posteriorly.
4. Elevate a periosteal pocket to accommodate the implant coil.
5. Elevate a narrow periosteal pocket against the bone under the temporalis muscle. This is to make a place for the extracochlear electrode between the skull and the periosteum, i.e. under the temporalis muscle.

4. Mastoidectomy and preparing the bone recess

The cortical mastoidectomy is described next. Some surgeons prefer to drill the implant recess first.

The cortical mastoidectomy

Create an adequate cortical mastoidectomy cavity, allowing an overhang both superiorly and posteriorly to accommodate any redundant proximal electrode lead.



Note

For children, it is recommended that a mastoidectomy be performed.

The bone recess

The blue dye dot on the bone indicates the position of the channel for the electrode lead exit.

Use the Recess Gauge, Bone Recess Template, Implant Template or the Sterile Silicone Implant Template to determine the angular orientation of the implant. This is usually placed at 30 to 45 degrees above the temporal line.



Warning

When drilling the bone recess, take care to avoid injury to the underlying dura.

To drill the bone recess:

1. Mark the recess using a surgical marker with the aid of the Recess Gauge, Implant Template, or the Sterile Silicone Implant Template.
2. Drill the bone recess. Aim to achieve a flat surface 'ramp', starting deeper on the anterior end of the implant and tapering off posteriorly. The ramp should be approximately 2.2 mm deep at the antero-inferior end of the implant, depending on the thickness of the skull. Providing that the skull is sufficiently thick, drilling deeper will result in a lower profile beneath the skin flap.

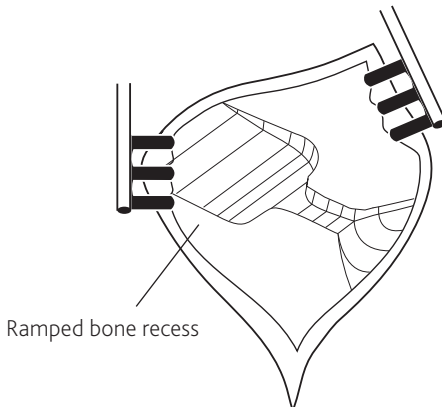


Figure 6: Ramped bone recess

3. Check the final dimensions of the bone recess using the Recess Gauge or Implant Template.

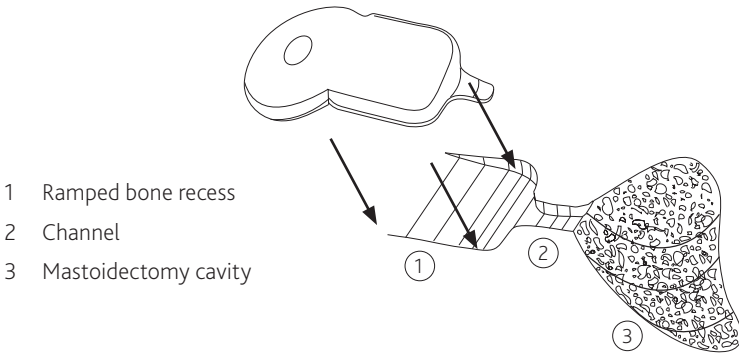


Figure 7: Ramped bone recess, electrode channel and mastoidectomy

4. Place the Implant Template or Recess Gauge in the bone recess and use it to mark the exit of the electrode.
5. Drill a channel to connect the bone recess and mastoid cavity — see *Figure 7* above. The channel will help protect the electrode against trauma.
6. Use the Recess Gauge to check the position and depth of the electrode exit.

5. Drilling tie-down holes

1. Using the implant seat for orientation (see *The bone recess* on page 33), mark tie-down holes above and below the anterior portion of the receiver/stimulator to ensure the implant can be secured.
2. Drill these holes with a 2 mm diamond burr.

Note

For children, an elevator may be used to protect the dura.

For additional support, posterior tie-down holes may be drilled or the implant coil can be placed under a pericranium pocket.



Figure 8: Tie-down holes for CI600 Series implants



Warning

When drilling the tie-down holes, take care to avoid injury to the underlying dura.

6. Opening the facial recess (Posterior Tympanotomy)

1. Open the facial recess ensuring it gives as much visibility and access as possible. The horizontal canal and short process of the incus should be clearly visualised.
2. Identify the facial nerve and chorda tympani nerve, but do not expose them.

The posterior portion of the middle ear, including the stapedius tendon, promontory and round window niche (RWN), should be clearly visualised.

In some instances of poor round window visualisation, the chorda tympani nerve is unavoidably cut to perform an extended facial recess approach.

7. Preparing the round window or cochleostomy

The CI632 implant electrode is compatible with both the round window and cochleostomy approaches.

This section describes site preparation for both approaches. For details on inserting the electrode array see *11. Inserting the intracochlear electrode* on page 45.



Caution

The recommended cochlea opening is between 0.8 mm and 1.0 mm wide.

The Cochleostomy Sizing Tool can be used to check the size during drilling and the final size of the opening.

If the opening is larger than 1.4 mm, use the forceps holding the sheath handle to stabilise the sheath and ensure the stopper stays at the round window or cochleostomy opening.



Warning

To avoid residual hearing loss or vestibular issues, do not suction the perilymph.

Round window

1. Visualise the stapes to confirm the site of the round window, and visualise the round window membrane. It is approximately 2 mm inferior and slightly posterior to the oval window.

The round window membrane may be obscured by the overhang of the lateral margin of the niche. It may be necessary to drill away the overhang to see the round window membrane.

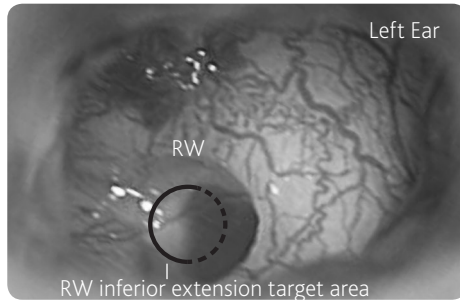


Figure 9: Round window target area

2. Remove the false membrane.



Warning

Do not open the round window membrane until immediately before insertion of the electrode as described in *11. Inserting the intracochlear electrode* on page 45.

Cochleostomy

1. Visualise the stapes to confirm the site of the round window, and visualise the round window membrane. It is approximately 2 mm inferior and slightly posterior to the oval window.
2. The round window membrane may be obscured by the overhang of the lateral margin of the niche and a mucosal false membrane. It may be necessary to gently drill away the overhang to see the round window membrane.
3. Perform a cochleostomy into the scala tympani using a diamond burr at low speed.
4. Position the cochleostomy inferior and slightly anterior to the round window membrane. It should be close to, or incorporating, the round window niche (RWN). A slight blue line of endosteum should become visible as the bone is being thinned for the cochleostomy. This indicates the location of the scala tympani.



Warning

Damage to the cochlea or vestibular system may be caused by drilling too far anteriorly or superiorly. This will result in the endosteum appearing white and the scala media or vestibuli may be entered.



Caution

Incorrect electrode placement may result from drilling too far inferiorly. This will miss the cochlea entirely and a hypotympanic air cell may be entered. Take care to remove bone dust, blood and other fluids from the cochleostomy.

5. Drill sufficient bone to expose at least 0.8–1.0 mm of endosteum.



Warning

To avoid risk of contamination do not open the endosteum until immediately before insertion of the electrode as described in *11. Inserting the intracochlear electrode* on page 45.

6. Remove the final layer of bone.

8. Inspecting the implant, electrodes and sizing tool

If the Sterile Silicone Implant Template is not unpacked see 2. *Opening the CI500 Series Sterile Silicone Implant Template* on page 31.

1. Remove the implant tray (white seal) from the packaging.
2. Tear open the seal of the implant tray and check the tray contains an implant and a Cochleostomy Sizing Tool.
3. Remove the implant.
4. Confirm the implant is not damaged and the electrode is contained within the sheath.



Warning

From this point, do not use monopolar electrosurgical instruments on the neck and head of the patient.

Bipolar electrosurgical instruments may be used; however the cautery electrode tips must not contact the cochlear implant and should be kept more than 1 cm (½ in) from the electrodes.



Caution

To avoid damage to the cochlear implant:

- minimise handling of the electrode
- do not bend the electrode as it is malleable and will deform
- leave the sheath on the electrode until just after insertion.

9. Positioning and securing the implant

1. Place the receiver/stimulator skin side up in the bone recess, with the implant coil in the subperiosteal/pericranial pocket between the tie-down holes.

For information on correct implant orientation see *Device description* on page 16.

2. Place the electrode lead in the centre of the channel.
3. Secure the receiver/stimulator with a single suture, using a non-absorbable synthetic material.

Move the knot to the edge of the cochlear implant.



Note

Do not suture directly over the magnet cassette cover as this may obstruct potential cassette removal – see *Figure 23* on page 65.

10. Securing the extracochlear electrode

Carefully place the extracochlear electrode against the bone under the temporalis muscle.



Caution

To avoid mechanical stress on the electrode lead, do not place the extracochlear electrode in the temporalis muscle.

11. Inserting the intracochlear electrode

Before insertion

The following should be performed immediately before inserting the electrode.

Round window

Make a straight incision the width of the round window.

Cochleostomy

1. Open the endosteum with an otologic hook and ensure that the cochleostomy is wide enough to accommodate the electrode.
2. Remove any sharp edge of bone which might snag the electrode.



Warning

To avoid residual hearing loss or vestibular issues, do not suction the perilymph.

Overview of insertion steps



Figure 10: Steps for inserting electrode into the cochlea



Note

To prevent movement of the electrode in the cochlea:

- Before the insertion, ensure the lead is not twisted or coiled.
- Hold the sheath handle in forceps to introduce the electrode into the cochlea.
- Maintain hold and control of the electrode until it is fully inserted, the sheath is removed and the lead is stabilised.



Caution

If resistance is felt during insertion, stop immediately, withdraw the sheath and assess the exposure of the round window or cochleostomy opening. You should be able to advance the electrode without resistance. Do not use force.



Warning

If the cochleostomy or round window incision is wider than 1.4 mm or significant resistance is felt during array insertion, use both hands to stabilise before continuing. This will help prevent the sheath stopper advancing through the opening.

Insertion

To insert the intracochlear electrode into the cochlea:

- A. Hold the sizing tool by the handle with AOS Forceps. Insert the sizing tool into the cochleostomy or round window opening until the silicone stopper reaches the cochlea opening. Ensure that the tip of the sizing tool easily enters the cochlea opening and the stopper doesn't advance through the opening.
This is to check the cochlea opening width is between 0.8 mm and 1.0 mm.
- B. Put the sizing tool down. Use blunt-nosed forceps with serrated tips to take hold of the electrode by the sheath handle.
- C. Holding the sheath handle securely, use AOS Forceps to gently hold the electrode lead below the white alignment marker as shown. To straighten the intracochlear electrode, slowly retract the electrode until it is fully inside the sheath and resistance is encountered.

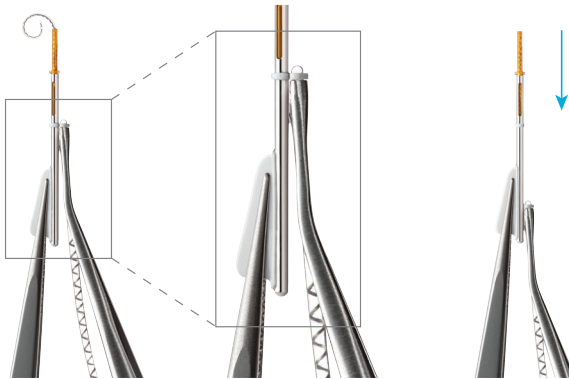


Figure 11: Straightening the intracochlear electrode

- D. Hold the sheath handle with forceps and direct the sheath and electrode array towards the opening of the cochleostomy or round window. Orientate the sheath handle toward the modiolus so the electrode curve follows the cochlea spiral, ensuring it is guided through the scala tympani with stimulating pads facing the modiolus. Guide the sheath into the cochlea until the sheath stopper reaches the cochleostomy or round window.

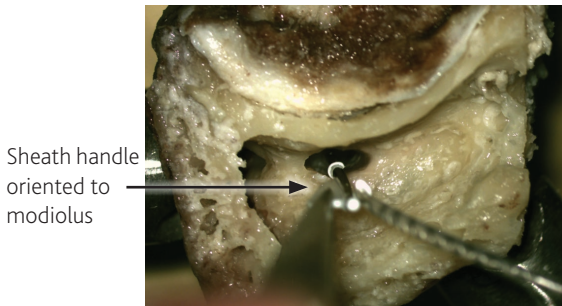


Figure 12: Inserting sheath tip into cochleostomy or round window opening (right ear temporal bone shown)



Caution

If resistance is felt during insertion, stop immediately, withdraw the sheath and assess the exposure of the round window or cochleostomy opening. You should be able to insert the sheath to the stopper without resistance. Do not use force.



Note

Ensure correct orientation of the electrode in the scala tympani.

- Use the white sheath handle as a guide for correct orientation. The handle should be orientated towards the modiolus and follow the plane of the scala tympani.
- If the handle is not aligned correctly, the electrode tip could move down towards the floor of the scala tympani or up towards the basilar membrane, meaning electrode placement will be sub-optimal with compromised positioning in the scala tympani.
- Be aware of the lead coiling from the electrode to receiver/stimulator as this could also impact electrode direction.

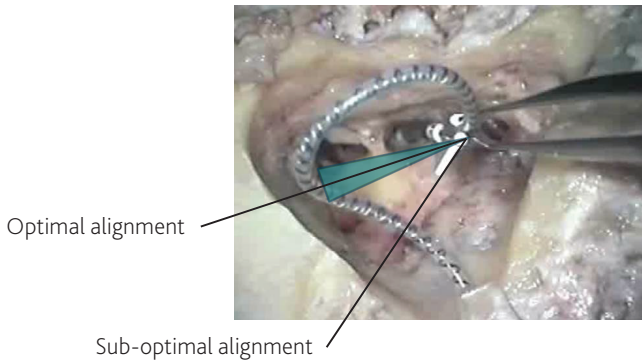


Figure 13: Aligning handle along medial plane of scala tympani



Note

Ensure the electrode remains in the sheath during insertion.

- During insertion, **do not** hold the electrode to insert the sheath up to the stopper.
- Hold only the sheath handle until the stopper is at the cochleostomy or round window entrance. Then use your other hand to advance the electrode through the sheath.
- This can prevent the electrode tip from prematurely advancing from the sheath before the stopper is correctly positioned against the cochlea opening.



Figure 14: Electrode tip visible from end of sheath before reaching cochleostomy entrance



Warning

Ensure the sheath stopper remains against the cochleostomy or round window opening.

- Ensure the sheath stopper is at the cochleostomy or round window. If the electrode is advanced before the stopper reaches the cochleostomy or round window, the tip could fold over.
- If the cochleostomy or round window opening is too large, use AOS Forceps to hold the electrode and, with your other hand, use forceps to stabilise the sheath stopper at the entrance to prevent the stopper being pushed too far.

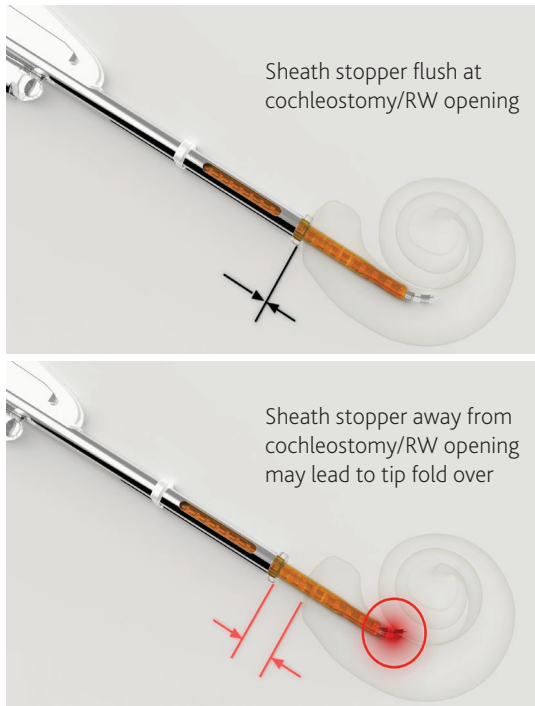


Figure 15: Sheath not flush at cochleostomy entrance may result in poor insertion

- E. Continuing to hold the sheath handle, use AOS Forceps to grip the electrode lead behind the white marker. Use AOS Forceps to advance the electrode through the sheath guide tube until the white markers are aligned.

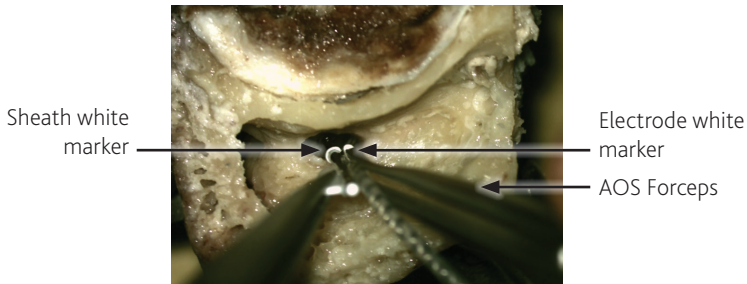


Figure 16: Advancing electrode into cochlea
(right ear temporal bone shown)

The electrode array is now fully inserted into the cochlea but the sheath is still attached to the electrode lead.



Caution

If resistance is felt before full insertion, stop immediately and assess the trajectory and/or position of the sheath. You should be able to advance the electrode without resistance. Do not use force.

- F. While continuing to hold the electrode lead with AOS Forceps, use forceps to slowly retract the sheath, sliding it straight back in line with the electrode array until completely disengaged.

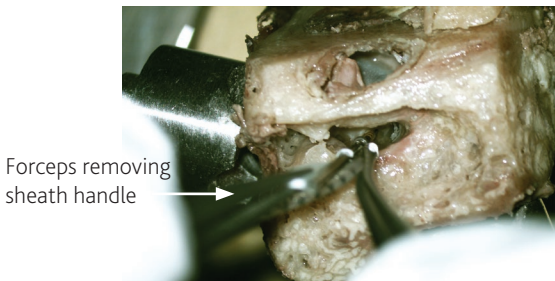


Figure 17: Removing sheath with forceps

- G. The electrode is fully inserted in the cochlea with the sheath removed. The three white insertion depth markers can be used to confirm the inserted depth of the electrode. If the three markers are at the cochleostomy or round window opening, a full insertion has been performed.

Ensure the array is not pushed or advanced further into the cochlea to avoid over-insertion and compromised perimodiolar positioning.

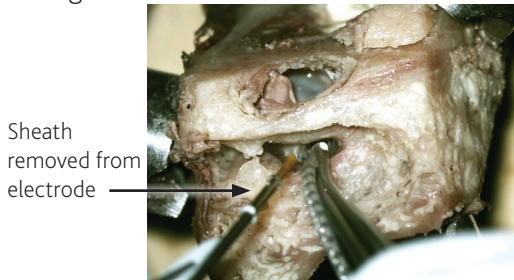


Figure 18: Electrode array fully inserted into cochlea and sheath removed



Warning

- Ensure the sheath is fully removed. The sheath needs to be completely removed from the electrode and **not** left in place after the procedure is complete.
- Keep the sheath in the sterile field in case it is needed for a second insertion attempt. See *Reloading the sheath* on page 54.

Reloading the sheath

If electrode placement is suboptimal or the sheath is removed prematurely, the electrode may be reloaded into the sheath for a second insertion attempt.



Warning

Reload only if the electrode and sheath are undamaged. If damage is identified use the backup implant; do not attempt reload.

1. Hold the sheath handle with forceps and gently hold the electrode lead with AOS Forceps below the white alignment mark, as shown below.
2. Guide the proximal electrode gently into the tip of the sheath.
3. When the electrode base is in the tip of the sheath, slowly retract the electrode array until resistance is encountered (ready for insertion into the cochlea).

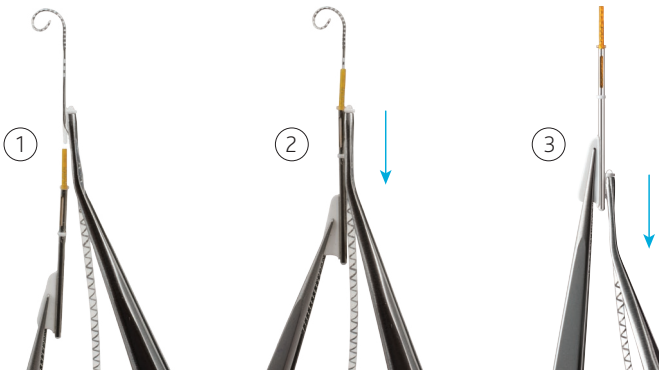


Figure 19: Guiding the electrode into sheath and retracting the electrode array



Caution

Check that the electrode is fully contained within the sheath. If not, push the electrode entirely out and repeat from step 1.

12. Securing and sealing the intracochlear electrode



Warning

Movement of the excess electrode lead could result in the electrode twisting and potentially damaging cochlear structures. Immediately after inserting the electrode and before arranging the excess proximal electrode lead in the mastoid cavity, the electrode must be immobilised. Ensure the electrode is held in place continuously.

To limit the risk of migration or breaking the seal, the electrode may be secured. The method of fixation, and choice of fixation points, will depend on surgical access and the surgeon's discretion.

1. Pack completely around the electrode in the cochleostomy or round window with an autograft consisting of strips of fascia or pericranium to ensure there are no gaps in the seal.



Note

If there is a perilymph leak, extra tissue may be needed to ensure that the seal is tight.

2. Coil the excess redundant proximal electrode lead inside the mastoid cavity under the bony overhangs.
3. Place any excess loop of the extracochlear electrode in the mastoid cavity.



Note

If the electrodes are able to migrate into subcutaneous tissue they may be subject to excessive movement and fatigue. To avoid this, ensure the leads are secure within the cavity, but do not suture over the electrode leads with fine gauge sutures.

Confirmation of electrode placement

Before closure, an X-ray may be obtained (preferably a lateral or modified Stenver's view) to confirm proper electrode placement.

For information on Stenver's view, contact Cochlear or see Xu J, Xu SA, Cohen LT, Clark GM. Cochlear View: Post-operative Radiography for Cochlear Implantation. Am J Otol, 21(1):49-56, 2000.

13. Performing intraoperative measurements

Intraoperative measurements via telemetry may now be performed.

1. Replace the flap.
2. Put the processor coil and cable in a sterile sleeve.



Warning

If using the Intraoperative Spacer, place the coil on top of the Intraoperative Spacer in the sterile sleeve.

3. Place the external coil over the implant magnet.



Note

- The transmitting range of the cochlear implant is 1 mm to 10 mm. However, a maximum skin flap thickness of 6 mm to 10 mm is required for good magnet retention.
- The cochlear implant may not function properly if the processor coil is placed directly on top of the receiver/stimulator.
- Methods to determine that the cochlear implant is functioning properly include impedance measurement using a Cochlear proprietary programming system.

14. Closure

1. Pack the facial recess with soft tissue.
2. Suture the palva flap over the proximal portion of the intracochlear electrode lead.
3. Close the wound in layers. Drainage is not recommended.
4. Apply a large mastoid pressure dressing.

Post-operative management

Monitor the patient as for all procedures involving general anaesthesia. Keep the pressure dressing on for one day, then inspect the wound and apply another dressing for five days.

Fitting the sound processor

The initial fitting procedure for the sound processor should be scheduled three to four weeks after the operation. Fitting should be checked at three months, six months and one year postoperatively, then at yearly intervals (or more frequently if required by the condition of the patient).

Registering the implant

Registration form

Complete the registration form. Send the completed form to Cochlear within 30 days of receiving the product.

Patient identification card

Fill out the implant model number and ear details on the patient identification card. Give the card to the patient or their carer.

The patient or their carer should carry the patient identification card with them at all times.

Identifying the implant

For information on identifying Cochlear implants without surgical intervention, refer to the *Cochlear Nucleus Implants MRI Guidelines*.

Explanting the implant

In rare circumstances, it may be necessary to explant a cochlear implant. Please follow the steps below.

1. Contact Cochlear to order a Retrieved Device Kit. The kit must be used to transport the explanted device to Cochlear.
2. Read the instructions provided with the kit.
3. Before explanting the device, examine it for any defects. Note these on the form provided with the kit.
4. Try to keep the explanted device intact and undamaged. To assist in removing the device undamaged you can cut the intracochlear electrode lead. See *Cutting the intracochlear electrode lead* on page 61.
5. If the intracochlear electrode lead is removed from the cochlea, place it in the kit, even if it is damaged.
6. Return the kit containing the explanted device to the Cochlear address nearest you.

Cutting the intracochlear electrode lead

Cut the intracochlear electrode lead if it will assist you to remove the device without damaging it. The cut should be in the region of the electrode lead shown below.

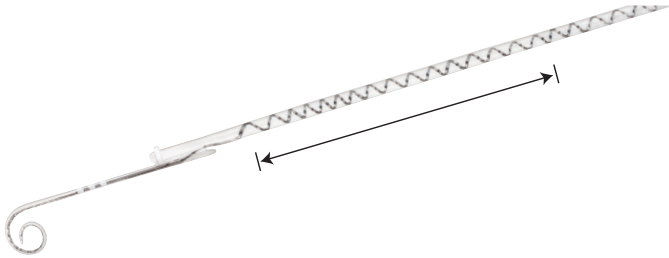


Figure 20: Where to cut electrode lead if required during explantation

Reporting problems

Legislation on medical devices requires the manufacturer to report adverse events to the appropriate authorities. Should such an incident occur, notify the nearest Cochlear office or its official distributor as soon as possible.

MRI safety information



The Cochlear Nucleus CI632 cochlear implant is MR Conditional. MRI examinations can be performed safely on a person with this implanted device only under very specific conditions. MRI examinations performed under different conditions may result in severe patient injury or device malfunction.

Full MRI safety information is available:

- in the *Cochlear Nucleus Implants MRI Guidelines*
- by visiting www.cochlear.com/warnings
- by calling your regional Cochlear office – contact numbers are available on the back cover of this guide.



All external components of the Cochlear implant system (e.g. sound processors, remote assistants and related accessories) are MR Unsafe. The patient must remove all external components of their Cochlear implant system before entering a room where an MRI scanner is located.

Removing the magnet cassette

Cochlear Nucleus CI600 Series implants are designed to withstand MRI at static magnetic field strengths described in the *Cochlear Nucleus Implants MRI Guidelines*.

Before an MRI examination, in some instances the magnet cassette must be removed in a sterile surgical environment. If single or multiple MRI examinations on the head are needed with the magnet cassette removed, replace the magnet cassette with a non-magnetic cassette.



Warning

To prevent infection, do not leave the magnet pocket empty. When removing the magnet cassette, replace the magnet cassette with a non-magnetic cassette.



Caution

When removing or inserting a magnet cassette or non-magnetic cassette:

- Take care to not damage the implant silicone or coil wires.
- Minimise force applied to the implant and electrodes.
- Minimise pressure applied to the implant coil.



Note

While the magnet cassette is removed, the recipient must wear a retainer disc to hold their sound processor coil in place. Retainer discs are available from Cochlear.

Replacement magnet cassettes and non-magnetic cassettes



Warning

To avoid implant damage during an MRI examination and potential revision surgery, ensure CI600 Series magnet cassettes and non-magnetic cassettes are used.

Do not use magnets and non-magnetic plugs for other implants, such as CI500 and CI24RE Series.

Replacement magnet cassettes and non-magnetic cassettes are available from Cochlear.



Figure 21: Nucleus Replacement Magnet Cassette – P782485



Figure 22: Nucleus Non-Magnetic Cassette – P782484

Removing the magnet cassette before implantation

If an MRI examination is scheduled in the near future, it may be appropriate to replace the magnet cassette with a non-magnetic cassette before the device is implanted.

The replacement procedure should take place under sterile conditions.

Replacing magnet cassette with non-magnetic cassette before implantation

1. In sterile conditions, remove the implant from its sterile packaging and place it on a flat and stable surface with the bone side (engraved side) facing down.

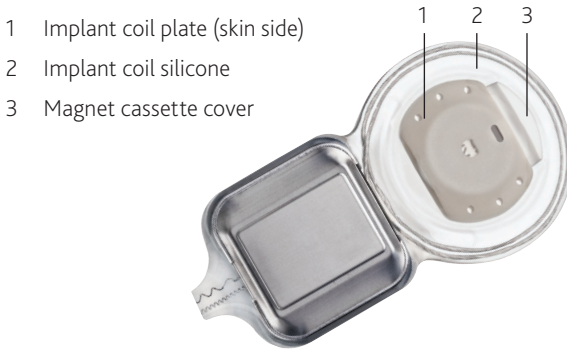


Figure 23: CI632 implant with magnet cassette



Warning

To avoid infection, if the sterile package or implant are damaged do not use the implant.

2. At the distal end of the implant coil, carefully position forceps or similar instrument under the silicone lip to hold the centre of the magnet cassette cover.

- 1 Silicone lip
- 2 Forceps tip under silicone lip
- 3 Magnet cassette cover

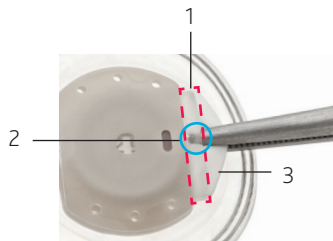


Figure 24: Forceps position on CI632 magnet cassette cover



Caution

When holding the magnet cassette cover, take care not to damage the silicone lip or the silicone around the magnet pocket opening.

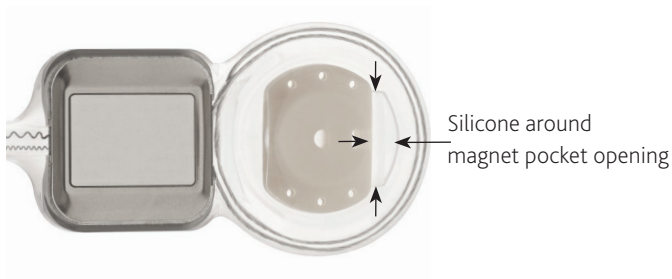


Figure 25: CI632 implant with magnet cassette removed

3. Using constant traction, remove the magnet cassette from the magnet pocket. The magnet cassette cover is designed to stretch under the constant traction applied during removal.

The removal direction is in the same plane as the implant coil, towards the distal end of the implant – see arrow in *Figure 26* below.



Caution

To avoid damaging the magnet pocket, do not apply vertical pulling force to the implant coil.



Figure 26: CI632 implant with magnet cassette partially removed



Note

If the magnet cassette cover pulls away, use forceps to hold the metal tab and continue removal.



Figure 27: Metal tab on magnet cassette



Figure 28: CI632 implant, magnet cassette removal using metal tab

4. Dispose of the removed magnet cassette. It is not re-usable.
5. To insert the sterile non-magnetic cassette into the magnet pocket, remove it from the packaging and silicone carrier. Ensure the MRI engraving is facing up (skin side).



Warning

To avoid infection, if the sterile package is damaged do not use the non-magnetic cassette.

Insert the non-magnetic cassette into the magnet pocket between the implant coil plates, being careful not to exert undue force or pressure on the implant or implant coil.

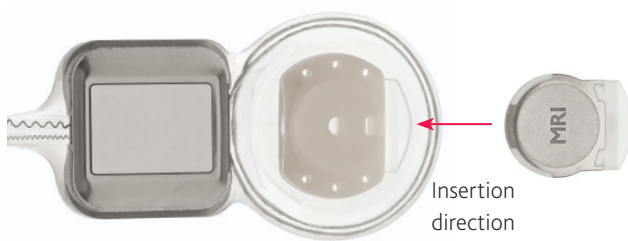


Figure 29: Non-magnetic cassette insertion direction

6. Ensure the non-magnetic cassette is fully inserted into the magnet pocket and the non-magnetic cassette cover is flush with the surrounding implant silicone.

The implant is now ready for implantation.

When there is no further need for MRI examinations, replace the non-magnetic cassette as instructed in *Removing and replacing the magnet cassette or non-magnetic cassette after implantation* on page 70.

Removing and replacing the magnet cassette or non-magnetic cassette after implantation



Warning

Do not use vertical force. Take care not to displace the implant.

Use of excessive or vertical force could lead to implant or electrode migration, causing the implant to malfunction and require removal, replacement or revision surgery.



Caution

- Take care not to damage the implant silicone or coil wires.
- When holding the magnet cassette cover or non-magnetic cassette cover, take care not to damage the silicone lip or the silicone around the magnet pocket opening.



Note

The magnet cassette or non-magnetic cassette can be safely removed and replaced with a new sterile magnet cassette or non-magnetic cassette up to eight times without any adverse effect to the implant.

Remove the magnet cassette or non-magnetic cassette in sterile conditions, using either general or local anaesthetic.

1. Make an incision beyond the distal end of the implant coil.



Note

You may use the cassette's silicone carrier to mark the incision:

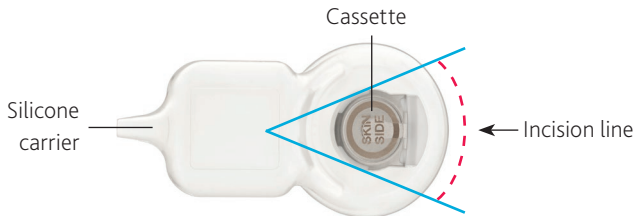


Figure 30: Marking the incision using the silicone carrier

2. Cut through any fibrous growth around the implant, exposing the distal end of the implant coil and the cassette cover. Ensure there is good visibility and access to the cassette cover.
3. Stabilise the implant, taking care to minimise force applied to the implant coil.
4. At the distal end of the implant coil, carefully position forceps or similar instrument under the silicone lip to hold the centre of the cassette cover.

- 1 Silicone lip
- 2 Forceps tip under silicone lip
- 3 Cassette cover

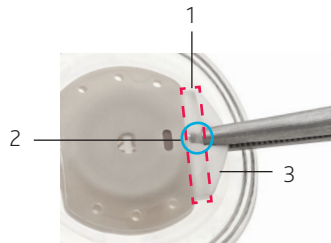


Figure 31: Forceps position on CI632 implant, cassette cover

5. Using constant traction, remove the magnet cassette or non-magnetic cassette from the magnet pocket. The removal direction is in the same plane as the implant coil, towards the distal end of the implant – see arrow in *Figure 32* below.



Note

The magnet cassette and non-magnetic cassette have been designed to remain in place and not move during an MRI examination. Therefore additional force may be required to remove the magnet cassette or non-magnetic cassette. In such cases, ensure the implant is sufficiently stabilised during removal.



Figure 32: CI632 implant with cassette partially removed

**Note**

If the cassette cover pulls away, use forceps to hold the metal tab and continue removal.



Figure 33: Metal tab on cassette



Figure 34: CI632 implant, cassette removal using metal tab

6. Dispose of the removed magnet cassette or non-magnetic cassette. They are not re-usable.

7. To insert a sterile replacement magnet cassette or non-magnetic cassette, remove it from the packaging and silicone carrier.

Ensure that:

- the engraving SKIN SIDE (or MRI) is facing up – see *Figure 35* below
- there is good visibility and access to the magnet pocket.



Warning

To avoid infection, if the sterile package is damaged do not use the replacement magnet cassette or non-magnetic cassette.

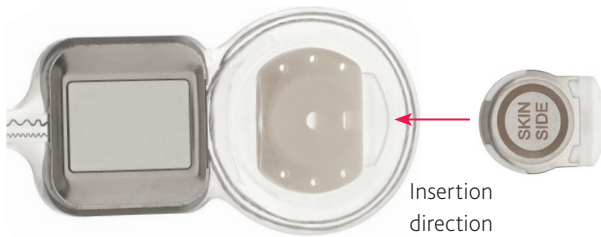


Figure 35: Replacement magnet cassette insertion direction

8. Stabilise the implant, taking care to minimise force applied to the implant coil.
9. Insert the replacement magnet cassette or non-magnetic cassette into the magnet pocket between the implant coil plates, being careful not to exert undue force or pressure on the implant or implant coil.

Ensure the replacement magnet cassette, or non-magnetic cassette, is fully inserted into the magnet pocket and the cassette cover is flush with the surrounding implant silicone.

10. Closure – close the wound in layers (drainage is not recommended) and apply a large pressure bandage.

How the implant is supplied

The implant, non-magnetic cassette and replacement magnet cassette are single-use items, not to be used more than once. Non-magnetic cassettes and replacement magnet cassettes are supplied separately.

All of the above components are supplied in sterile gas-permeable packaging. Ethylene oxide processing is indicated on the label of each sterile package.

Before opening the sterile package, inspect it carefully. Return the device and packaging to Cochlear if:

- the 'use by' date stamped on the outside package has expired
- the sterile package containing the implant is ruptured
- exposure to ethylene oxide processing is not indicated by a green dot on the sterile pack.

Transport and handling

Nucleus cochlear implants inside their sterile packaging within the implant box have been validated for transport and handling temperatures from -10 °C (+14 °F) to +55 °C (+131 °F).

Handle with care. Severe impact may rupture the sterile package inside.

Storage

Store Nucleus cochlear implants inside their sterile packaging within the implant box at room temperature. Keep dry.

CI632 implant specifications

Intracochlear electrodes

Number of electrodes	22 electrodes
Distance between centres of electrode contacts	0.6 mm nominal (when curled)
Cross-sectional dimensions of array	0.475 mm x 0.5 mm at proximal end, tapering to 0.35 mm x 0.4 mm at distal end
Contact surface area	0.15 mm ² to 0.16 mm ²
Active array length when straightened	14 mm (distance between most basal and apical electrodes)
Lead length	98 mm from receiver/stimulator to array tip when straightened
Markers for insertion depth	Three white, moulded silicone markers

Extracochlear electrodes

- Plate on receiver/stimulator
- Cylindrical electrode 0.6 mm (typical) diameter with hemispherical tip, on a lead 60 mm in length.

Receiver/Stimulator

Dimensions	Case: 24 mm x 23 mm x 3.9 mm Coil: 31 mm diameter x 3.9 mm thick
Volume	4.2 cm ³ without lead
Mass	9.2 g including electrode array

Operating characteristics

Power and data	Received by 5 MHz inductive link from sound processor headset coil
Current	Biphasic pulses
Stimulation mode	Monopolar, bipolar or common ground
Stimulus amplitudes	Programmable from 0 μ A to 1750 μ A nominal at 37 °C
Maximum stimulus amplitude	Median: 1750 μ A Range: 1575 μ A to 1925 μ A as measured according to EN 45502-2-3/ISO 14708-7
Output signal on a 1 k Ω resistor	Amplitude 1750 μ A, pulse width 400 μ s
Stimulus duration	Programmable from 9.6 μ s to 400 μ s per phase
Maximum stimulus pulse width	Median: 400 μ s Range: 398 μ s to 410 μ s as measured according to EN 45502-2-3/ISO 14708-7
Transmitting range	1 mm to 10 mm (6 mm to 10 mm maximum skin flap thickness required for good magnet retention)

Measurement functions

Compliance	Displays compliance limits using Cochlear proprietary programming software
Neural response telemetry	Measure of electrically evoked compound action potential (ECAP)
Impedance	Measure of electrode impedances in monopolar and common ground modes
Impedance measurement accuracy	80% measured according to EN 45502-2-3/ISO 14708-7
Implant ID and type check	Enables the sound processor to confirm whether it is coupled to the nominated implant

Materials in contact with body tissues

Silicone elastomer	Lead and receiver/stimulator protective coating and insulation Magnet cassette cover Non-magnetic cassette cover
Titanium	Receiver/stimulator case
Platinum	Electrode contacts

General information

Warranty

To the purchaser: the law in some countries requires that the written warranty for this cochlear implant must be made available for the patient's review before it is sold to them. The Cochlear terms and conditions of warranty should therefore be given to the patient before implantation of the cochlear implant. The warranty is included in the document pack.

Symbols

The following symbols may appear on your implant or implant packaging:



Fragile, handle with care



Do not use if package is damaged



Consult instructions for use



Refer to instruction manual



Specific warnings or precautions associated with the device, which are not otherwise found on the label



Do not re-use













Do not re-sterilise



Date of manufacture



Manufacturer

	Use-by date
	Keep dry
	Sterilised using ethylene oxide
Rx Only	Caution: US law restricts this device to sale by, or on the order of, a physician
	Catalogue number
	Serial number
	Batch code
	Authorised representative in the European Community
	CE registration mark with notified body number
	MR Conditional
	Medical Device
BONE SIDE	Bone side of implant, to be implanted with this side facing down
SKIN SIDE	Skin side of magnet cassette and replacement magnet cassette

Privacy and the collection of personal information

During the process of receiving a Cochlear device, personal information about the user/recipient or their parent, guardian, carer and hearing health professional will be collected for use by Cochlear and others involved in care with regard to the device.

For more information please read Cochlear's Privacy Policy on www.cochlear.com or request a copy from Cochlear at the address nearest you.

[illegible]

Hear now. And always

Cochlear Ltd (ABN 96 002 618 073) 1 University Avenue, Macquarie University, NSW 2109, Australia
Tel: +61 2 9428 6555 Fax: +61 2 9428 6352

Cochlear Ltd (ABN 96 002 618 073) 14 Mars Road, Lane Cove, NSW 2066, Australia
Tel: +61 2 9428 6555 Fax: +61 2 9428 6352

ECOREP Cochlear Deutschland GmbH & Co. KG Karl-Wiechert-Allee 76A, 30625 Hannover, Germany
Tel: +49 511 542 770 Fax: +49 511 542 7770

Cochlear Americas 10350 Park Meadows Drive, Lone Tree, CO 80124, USA
Tel: +1 303 790 9010 Fax: +1 303 792 9025

Cochlear Canada Inc 2500-120 Adelaide Street West, Toronto, ON M5H 1T1, Canada
Tel: +1 416 972 5082 Fax: +1 416 972 5083

Cochlear AG EMEA Headquarters, Peter Merian-Weg 4, 4052 Basel, Switzerland
Tel: +41 61 205 8204 Fax: +41 61 205 8205

Cochlear Europe Ltd 6 Dashwood Lang Road, Bourne Business Park, Addlestone, Surrey KT15 2HJ, United Kingdom
Tel: +44 1932 26 3400 Fax: +44 1932 26 3426

Cochlear Benelux NV Schaliënhoedreef 20 i, B-2800 Mechelen, Belgium
Tel: +32 15 79 55 11 Fax: +32 15 79 55 70

Cochlear France S.A.S. 135 Route de Saint-Simon, 31035 Toulouse, France
Tel: +33 5 34 63 85 85 (International) or 0805 200 016 (National) Fax: +33 5 34 63 85 80

Cochlear Italia S.r.l. Via Larga 33, 40138 Bologna, Italy
Tel: +39 051 601 53 11 Fax: +39 051 39 20 62

Cochlear Nordic AB Konstruktionsvägen 14, 435 33 Mölnlycke, Sweden
Tel: +46 31 335 14 61 Fax: +46 31 335 14 60

Cochlear Tibbi Cihazlar ve Sağlık Hizmetleri Ltd. Şti.
Çubuklu Mah. Boğaziçi Cad., Boğaziçi Plaza No: 6/1, Kavacık, TR-34805 Beykoz-Istanbul, Turkey
Tel: +90 216 538 5900 Fax: +90 216 538 5919

Cochlear (HK) Limited Room 1404-1406, 14/F, Leighton Centre, 77 Leighton Road, Causeway Bay, Hong Kong
Tel: +852 2530 5773 Fax: +852 2530 5183

Cochlear Korea Ltd 1st floor, Cheongwon Building 33, Teheran-ro 8 gil, Gangnam-gu, Seoul, Korea
Tel: +82 2 533 4450 Fax: +82 2 533 8408

Cochlear Medical Device (Beijing) Co., Ltd
Unit 2608-2617, 26th Floor, No.9 Building, No.91 Jianguo Road, Chaoyang District, Beijing 100022, P.R. China
Tel: +86 10 5909 7800 Fax: +86 10 5909 7900

Cochlear Medical Device Company India Pvt. Ltd.
Ground Floor, Platina Building, Plot No C-59, G-Block, Bandra Kurla Complex, Bandra (E), Mumbai – 400 051, India
Tel: +91 22 6112 1111 Fax: +91 22 6112 1100

株式会社日本コクレア (Nihon Cochlear Co Ltd) 〒113-0033 東京都文京区本郷2-3-7 お茶の水元町ビル
Tel: +81 3 3817 0241 Fax: +81 3 3817 0245

Cochlear Middle East FZ-LLC
Dubai Healthcare City, Al Razi Building 64, Block A, Ground Floor, Offices IR1 and IR2, Dubai, United Arab Emirates
Tel: +971 4 818 4400 Fax: +971 4 361 8925

Cochlear Latinoamérica S.A.
International Business Park, Building 3835, Office 403, Panama Pacifico, Panama
Tel: +507 830 6220 Fax: +507 830 6218

Cochlear NZ Limited
Level 4, Takapuna Towers, 19-21 Como St, Takapuna, Auckland 0622, New Zealand
Tel: + 64 9 914 1983 Fax: 0800 886 036

www.cochlear.com

Cochlear implant systems are protected by one or more international patents.
The statements made in this guide are believed to be true and correct as of the date of publication.
However, specifications are subject to change without notice.

ACE, Advance Off-Stylet, AOS, AutoNRT, Autosensitivity, Beam, Bring Back the Beat, Button, Carina, Cochlear, コクレア, 코클리어, Cochlear SoftWear, Codacs, Contour, コントゥア, Contour Advance, Custom Sound, ESprit, Freedom, Hear now. And always, Hugfit, Hybrid, Invisible Hearing, Kanso, MET, MicroDrive, MP3000, myCochlear, mySmartSound, NRT, Nucleus, Osia, Outcome Focused Fitting, Off-Stylet, Profile, Slimline, SmartSound, Softpit, SPrint, True Wireless, the elliptical logo, and Whisper are either trademarks or registered trademarks of Cochlear Limited. Ardium, Baha, Baha SoftWear, BCDrive, DermalLock, EveryWear, Human Design, Piezo Power, SoundArc, Vistafix, and WindShield are either trademarks or registered trademarks of Cochlear Bone Anchored Solutions AB.

© Cochlear Limited 2021

