



Nucleus[®] Smart App

User Guide

for iPhone[®] and iPod touch[®]

Version 6.0

Symbols used in this guide



Note

Important information or advice.



Tip

Time saving hint.



Caution (no harm)

Special care to be taken to ensure safety and effectiveness.
Could cause damage to equipment.



Warning (harmful)

Potential safety hazards and serious adverse reactions.
Could cause harm to person.



Note

Images shown in this guide are example screens only and may differ to what you see on your iPhone or iPad. Use the instructions in this guide in conjunction with the corresponding screens on your iPhone or iPad to guide you through pairing.

Nucleus® Smart App is intended to allow you to make adjustments to your sound processor (such as changing volume or programs, and selecting audio sources), and to monitor battery levels and receive alerts for sound processor issues.

Nucleus Smart App is compatible with Cochlear™ Nucleus® 8 Sound Processors, Cochlear™ Nucleus® 7 Sound Processors and Cochlear™ Nucleus® Kanso® 2 Sound Processors.

Step		Page
1	Download the Nucleus® Smart App from the App Store® to your iPhone or iPod touch*	–
2	IMPORTANT! Pair your sound processor(s) to your device <i>Refer to the Pairing Guide for iPhone/iPod touch</i>	–
3	Run the Nucleus Smart App	5
4	Follow the instructions on the screen to log in and set up the app	–
5	Start using the app!	6

* The Cochlear Nucleus Smart App is available on App Store® and Google Play®. For compatibility information visit www.cochlear.com/compatibility

Contents

Pairing basics

Pair your sound processor(s)	4
Unpair your sound processor(s).....	4

Use

Run the Nucleus Smart App	5
Security requirements	5
Use Apple Watch.....	6
The home screen.....	8
Control one or two processor(s)	9
Adjust volume.....	11
Change program.....	12
Stream audio	13
Adjust streamed audio.....	14
Adjust sensitivity	15
Adjust bass and treble.....	16
Adjust master volume limit.....	17
Use ForwardFocus.....	18

Use (continued...)

Check status	20
Sound Check	22
Settings menu	26
Firmware updates	28
Remote check	30
Remote Assist	34
Troubleshoot	38
General information.....	39

For more information, refer to the *Sound Processor User Guide*.

Visit us online for tips, how-to videos and more:
www.cochlear.com/

Pair your sound processor(s)

You need to pair your sound processor(s) to your device (for example, iPhone, iPod touch), before you can use the app's communication and control features.



Note

You can pair your sound processor with up to 5 compatible devices, but you can only control it from one device at any time.



Warning

Consider security when connecting your sound processor to devices such as smartphones or tablets. Only connect to devices that are protected, for example password or PIN access control. Do not connect to devices that have had their operating system altered.

See the *Pairing Guide for iPhone/iPod touch* for step-by-step instructions.

Unpair your sound processor(s)


If you change your sound processor(s), for example if you receive a new sound processor from the repair centre, you need to:

- First **Unpair** the old sound processor(s),
- Then **Pair** the new sound processor(s).

See the *Pairing Guide for iPhone/iPod touch* for step-by-step instructions.

Run the Nucleus Smart App

1. Tap the **Nucleus Smart** icon to start the app.



2. **Set up the app.** The first time you run the app, a series of screens step you through setting it up.



Note

You will need to log in to the app using your Cochlear account.

Security requirements

While using the Nucleus Smart App, you should:

- use a strong password for your Cochlear account
- configure devices to lock automatically when inactive
- use devices with security PINs or passcodes
- keep the device operating system updated
- keep the Nucleus Smart App updated
- never use devices with unauthorised modifications to the operating system.



Note

If you change your device, you must log out and uninstall the Nucleus Smart App from your previous device. Use the *Settings menu* to logout (see page 26).

Use Apple Watch

The Nucleus Smart App can be used on your Apple Watch if your watch is paired with your iPhone.*

After installation and set up of the Nucleus Smart App on your iPhone, check your Apple Watch to see if the Nucleus Smart App has installed automatically. If not, use the Watch app on your iPhone to select and install the Nucleus Smart App.

To use the app on your Apple Watch:

- start the app on your iPhone.
- keep your Apple Watch close to your iPhone.


You can change available settings on your Apple Watch or your iPhone – a change on one will be reflected on the other.

If your iPhone is dimmed, app alerts will show on your Apple Watch.

If your iPhone is turned off, Apple Watch app displays a message.


* Nucleus Smart App functions on Apple Watch are unavailable in some areas. If unavailable, a message displays in the app on your Apple Watch.

If your iPhone is turned on but the app isn't running, Apple Watch displays this message:



A subset of Nucleus Smart App functions are available on your Apple Watch. Screens for Apple Watch are included where relevant on the following pages.


The home screen

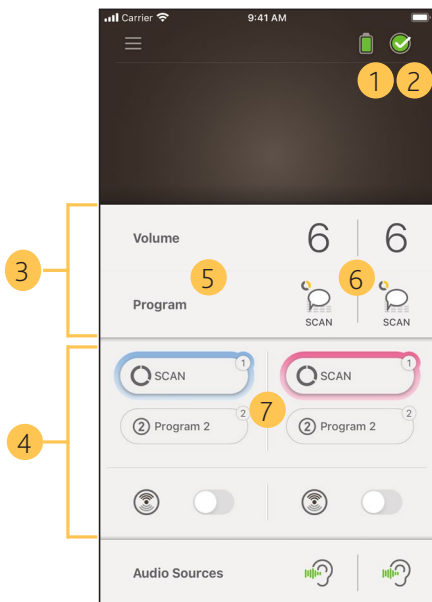

- 1 Sound processor battery level
- 2 Sound processor status
- 3 Control panel (closed)
- 4 Control panel (open)
- 5 Setting name
- 6 Setting current value
- 7 Setting controls

Control one or two processor(s)

You will see a green bar and one control if you only have one paired sound processor.

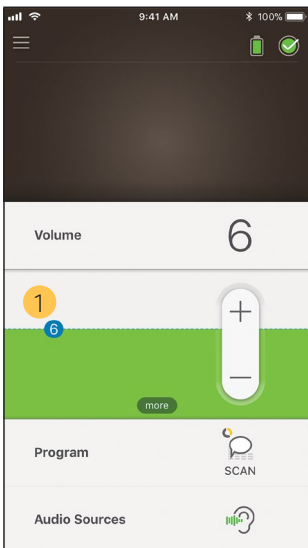


- 1 Default value (set by clinician). It may be different for each program, and for different sound processors.

If you have **two paired sound processors** you can control them together (one control button) or separately (two buttons, as shown here):

- Left side controls are blue
- Right side controls are red.



Change this using the *Settings menu* (see page 26).

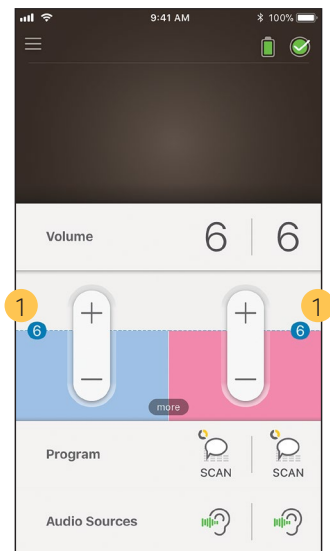

- 1 Default value (set by clinician). May be different for each program, and for different sound processors.



Adjust volume

1. Tap **Volume** to open its control panel.
2. Tap **+ / -** to change volume.

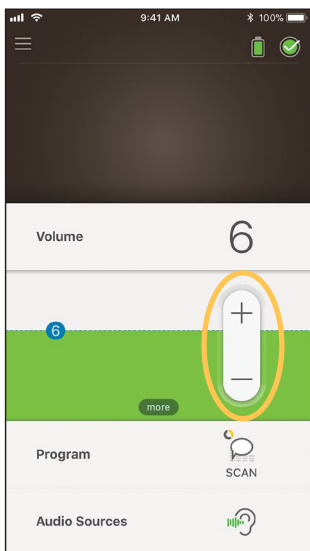


Change program

1. Tap **Program** to open its control panel.
2. Tap the icon for the program you want to use.

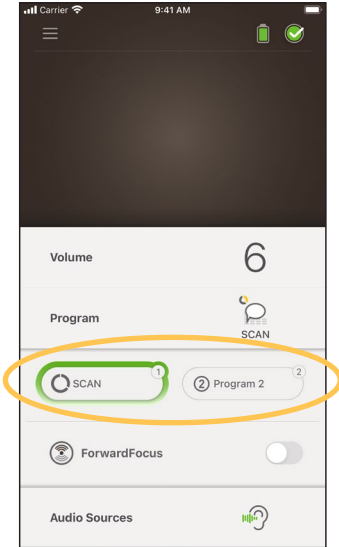

Stream audio

1. Tap **Audio Sources** to open its control panel.
2. Tap the **icon** for the audio source you want to use.

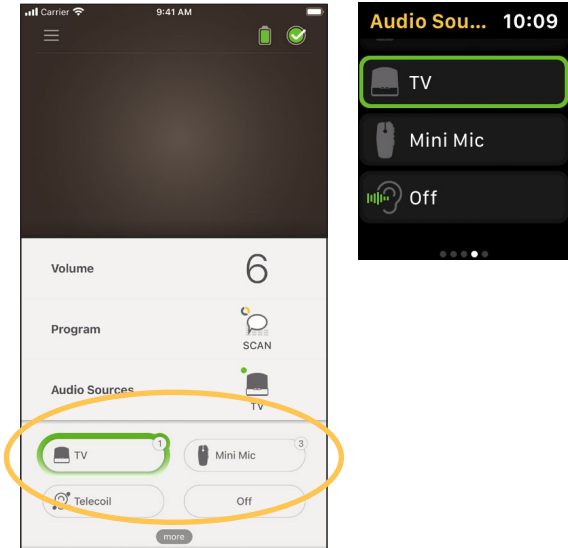

Tip

Tap **Off** or **X** to stop streaming audio and return to the previous program.

Adjust streamed audio



You can separately change the volume of the streamed audio and sound from your processor microphones.



Note

Audio Source Settings return to the default setting when you turn your sound processor off.

1. Start streaming from an Audio Source.
2. Tap **more** to open the **Audio Source Settings** control panel.
3. Tap **+ / -** to change settings.

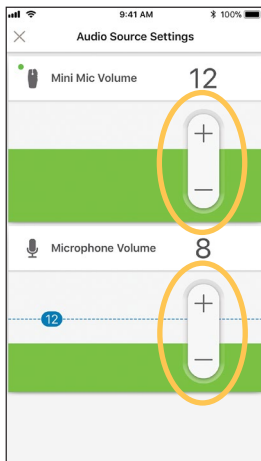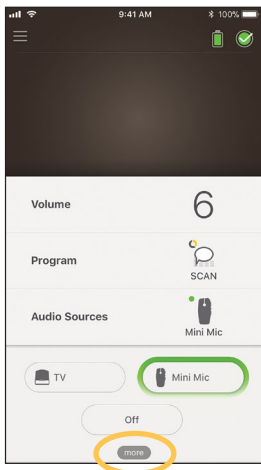

4. Tap **X** at top left to close the **Audio Source Settings** control panel.



Adjust sensitivity



Note

- Sensitivity is only available if enabled by your clinician.
- Sensitivity returns to the default setting when you turn your sound processor off.

1. Tap **Volume** to open its control panel.
2. Tap **more** to open the **mySmartSound** control panel.
3. Tap **+ / -** to change sensitivity.

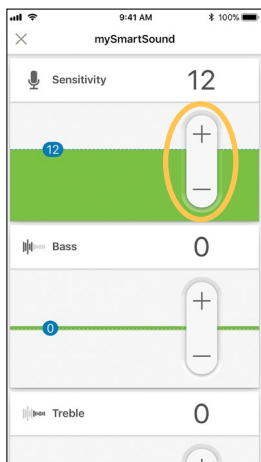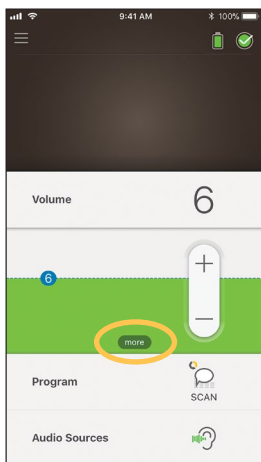

4. Tap **X** at top left to close the **mySmartSound** control panel.

Adjust bass and treble



Note



Bass and treble are only available if enabled by your clinician.



Warning

Only adjust this when you can hear sounds or speech. Increasing bass or treble may cause loud sounds or discomfort at high levels. If this occurs, remove the processor/coil immediately and decrease the bass or treble before replacing.

1. Tap **Volume** to open its control panel.
2. Tap **more** to open the **mySmartSound** control panel.
3. Tap **+ / -** to change bass or treble.

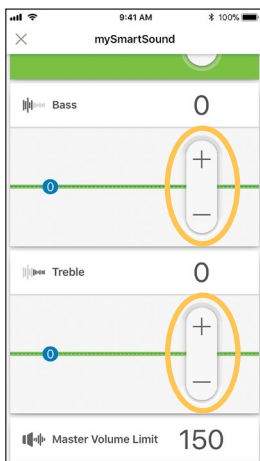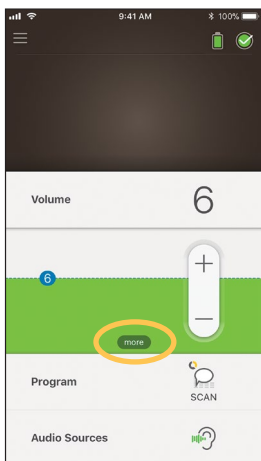

4. Tap **X** at top left to close the **mySmartSound** control panel.

Adjust master volume limit



Note



Master volume limit is only available if enabled by your clinician.



Warning

Only adjust this when you can hear sounds or speech. Increasing master volume limit may cause loud sounds or discomfort at high levels. If this occurs, remove the processor/coil immediately and decrease the master volume limit before replacing.

1. Tap **Volume** to open its control panel.
2. Tap **more** to open the **mySmartSound** control panel.
3. Tap **+ / -** to change master volume.

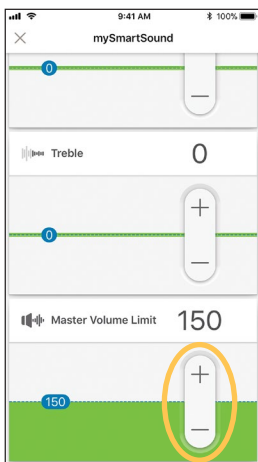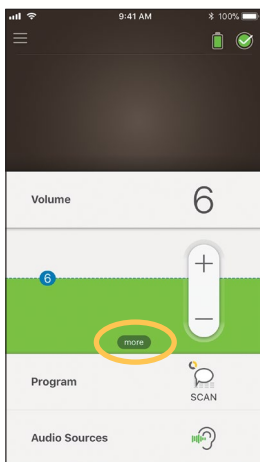

4. Tap **X** at top left to close the **mySmartSound** control panel.

Use ForwardFocus

ForwardFocus is an additional feature that works by reducing noise coming from behind you. This allows you to concentrate on face-to-face conversations in a noisy situation such as a café or noisy classroom.



Note

ForwardFocus is approved for users 12 and older and is only available if enabled by your clinician.

Once enabled, you have control of the feature and can turn it on and off as you need to.



Note

If you are using the program **SCAN 2 FF** on the Nucleus 8 Sound Processor, ForwardFocus is automatically managed by the program.

Only use ForwardFocus in noisy situations. When using ForwardFocus make sure any distracting noises are behind you.



Don't forget to turn it off when you move to a different hearing environment, for example, moving from a noisy café to a quiet room. If you notice a difficulty in understanding speech in a quiet setting, turn off ForwardFocus or request help from a caregiver.



Notes for caregivers

- If you are a caregiver of a child, you should talk to your clinician about the suitability of this feature. ForwardFocus should only be enabled for users 12 and older who are able to reliably provide feedback on sound quality and understand how to use the feature when moving to different or changing environments. It may be possible to have decreased speech understanding when using ForwardFocus in a quiet environment.
- It is important that your child understands they should not use ForwardFocus in quiet environments and that they should turn the feature off or provide feedback to a caregiver when ForwardFocus is no longer needed, and they need to use their normal programs.

1. Tap **Program** to open its control panel.
2. Turn **ForwardFocus** on.

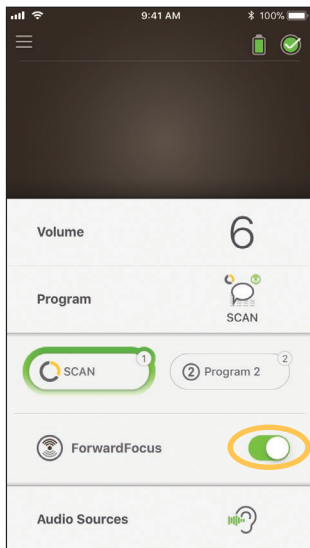

Note

- If you turn off your sound processor ForwardFocus is turned off and you will have to turn it on again when you need it.
- If you use an accessory or audio streaming, ForwardFocus is temporarily deactivated. ForwardFocus automatically resumes when you are no longer using an accessory or audio streaming.




Check status

Tap the icon to open the **Status** screen.





Note

Example screens show two sound processors. If you have one sound processor, your screens will show only that one.

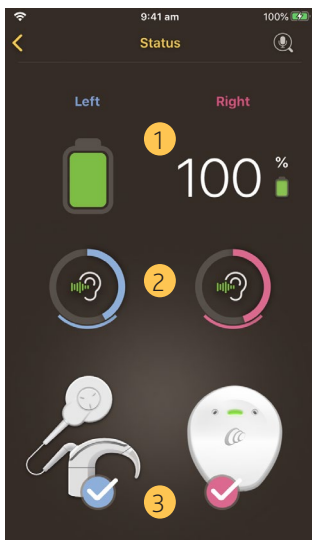

- 1 Sound processor battery level.
- 2 Sound level being delivered to the sound processor. Icon displays source (for example, microphones, telecoil, wireless accessory). Coloured bar indicates level.
- 3 Sound processor status indicator: Tick indicates no faults.

If your sound processor has a fault, you will see a screen like this:

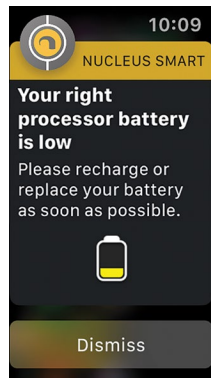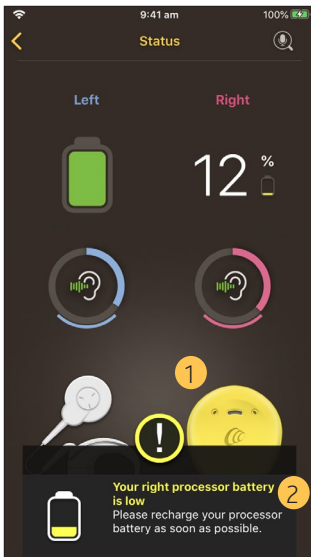

- 1 Sound processor part with the fault displays in yellow.
- 2 Description of fault and suggested solution.


Sound Check



Note

- Make sure you are in a quiet place away from microwave ovens, wireless routers or other devices that could cause interference.
- Place the smart phone near your processor with nothing in between like walls, furniture, your head.
- Be aware of privacy – Sound Check records sound from your processor microphone. Recordings are stored on your smart phone (they are not stored by Cochlear).

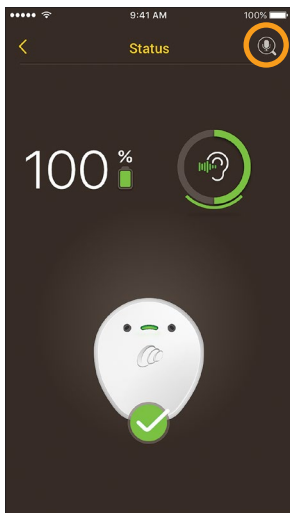

From the **Status** screen, tap the **microphone** icon to start Sound Check.*



* Only available with Kanso 2 Sound Processors and compatible smart phones. For information visit www.cochlear.com/compatibility.

1. If you have two processors, **Left** is selected. To record the right processor, tap **Right**.



2. Tap the **Microphone** button to start recording.
3. Tap the **Stop** button  to finish recording.
4. Tap the **Play** button  to listen to your recording.




Note

- While recording, the processor light displays steady blue.
- A 5-tone sequence sounds at the start of recording and 1 beep at the end.
- 30 seconds is the maximum recording time.
- Elapsed recording time displays above the button.
- The quality of speakers on your smart phone and headphones will affect the sound quality on playback.

Settings menu

Tap the **menu** icon at top left of the screen to open the **Settings** menu.

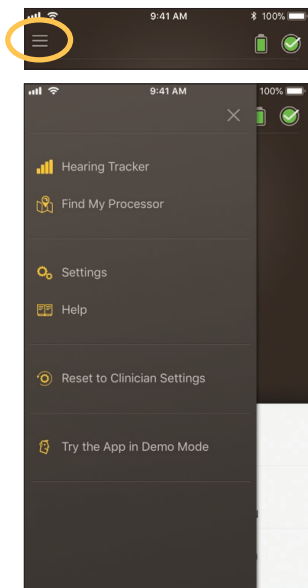


Tap **Reset to Clinician Settings** to change your processor settings back to those set by your clinician.

Tap **Try the App in Demo Mode** to learn how to use the app without affecting your processor(s).*

Tap **Settings** to open the **Settings** screen:

* This feature may not be available in your version of the app.

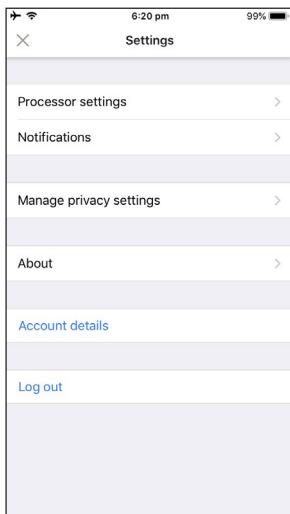

Tap **Processor settings** to:

- Set processor lights
- Turn beeps on/off.

Tap **Notifications** to turn notifications on/off.

Tap **Bilateral control** to select whether to control two sound processors together or separately.*

Tap **About** to view implant, processor and app information.

* This feature may not be available in your version of the app.

Firmware updates

The Nucleus Smart App automatically checks for firmware updates. Regular firmware updates will improve your sound processor's performance.

You need internet access to update the firmware. The update occurs after you confirm to proceed.




Note

Firmware updates may not be available in all areas.


When a firmware update is available, a message displays: A firmware update is available to help keep your sound processor running smoothly. Follow the prompts to complete the firmware update.

To manually check if a firmware update is available:

1. Tap the **menu** icon at top left of the screen, then tap **Settings**.

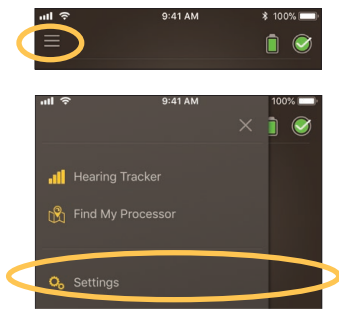

2. If a firmware update is available, tap the **Firmware update** option to perform the update.

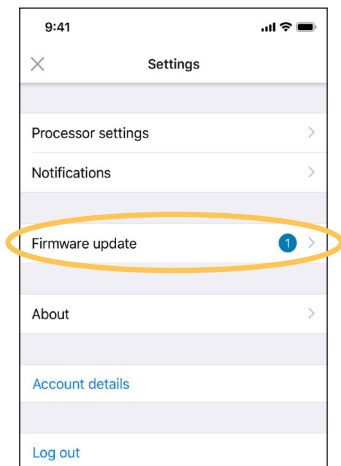

3. Follow the prompts to complete the firmware update process. For the firmware update to take effect you must restart your sound processor.

On successful update, a message displays:
Your firmware is now up-to-date on your sound processors!



Note

If the firmware fails to download or install correctly, the previous firmware version will be restored. The performance of your sound processor will not be affected if the update is unsuccessful.

Remote check

Remote Check is intended for ages 6 and older.



Remote Check allows you to complete a series of hearing tests using the Nucleus Smart App, then electronically send the results to your clinician for review.



Note


Remote Check must be enabled by your clinician.


1. Tap the **menu** icon at top left of the screen to open the **Settings** menu.

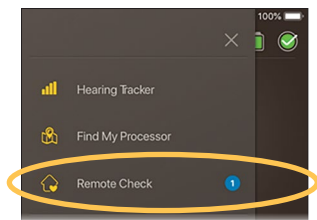


2. Tap **Remote Check** to see if it is time to start a Remote Check.

3. If it is time to start your Remote Check, tap **Get started**.

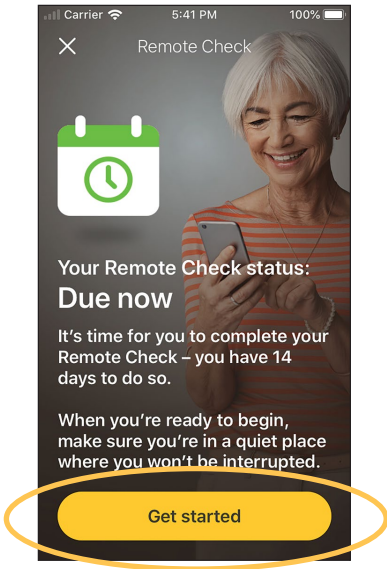


 **Note**
If you experience any discomfort during Remote Check, remove your processor/coil.

If it is not time to start your Remote Check, as determined by your clinician, a message will display saying 'You are not due for a Remote Check'.

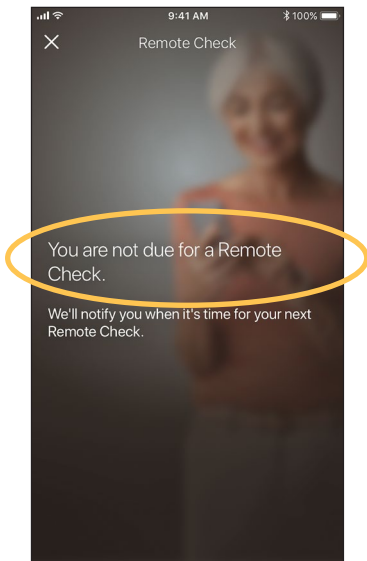

There are up to six steps in the Remote Check process. Follow the screen prompts to complete each step.

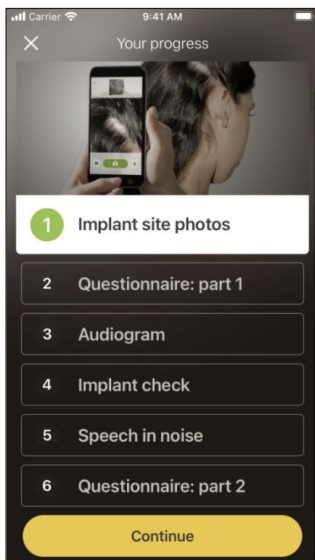

After you have completed the five steps your results will be sent automatically to your clinician.

Your clinician will review your results and notify you of any follow-up actions.

Remote Assist

Remote Assist is intended for ages 6 and older.

Remote Assist allows pre-scheduled video calls with your clinician so you can attend appointments remotely.



During the video call, your clinician is able adjust your sound processor settings. They will be unable to access any other settings or apps on your phone.




Note

- Remote Assist must be enabled by your clinician.
- Before the session, make sure your phone battery and sound processor battery are charged.

1. Tap the **menu** icon at top left of the screen to open the **Settings** menu.

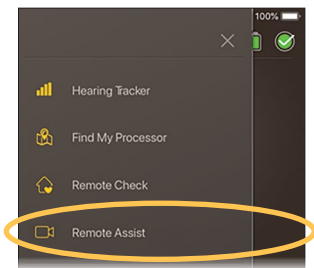

2. Tap **Remote Assist**.
3. When it's time for your Remote Assist appointment, tap **Get started**.

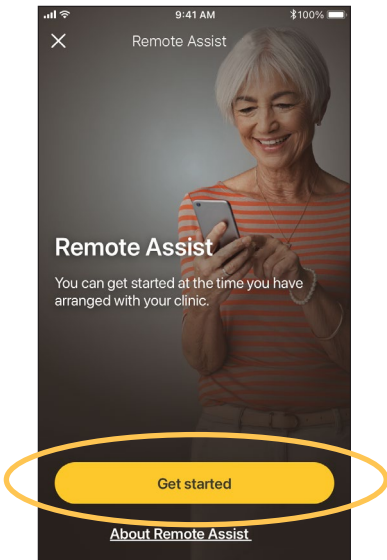

Note


If you experience any discomfort during Remote Assist, remove your processor/coil.

- When asked to provide microphone and camera access, tap **Allow** and **Continue**.



Note


Microphone and camera access are required to enable the call.

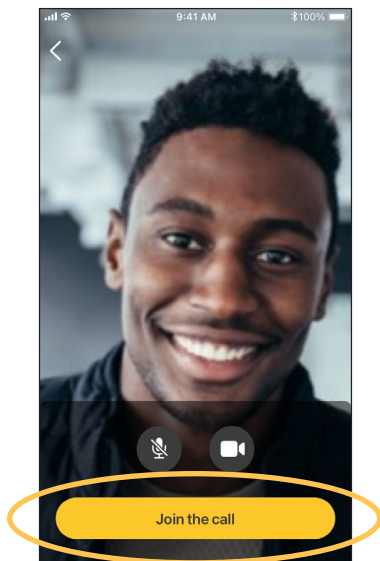

- Tap **Join the call** to attend your Remote Assist appointment.

If your clinician is not on the call, wait for them to join.

If your clinician makes changes to your sound processor, a status message displays at the top of the screen.

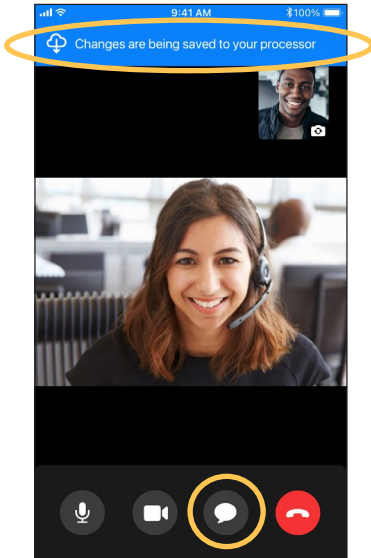

If you need to send a message to your clinician, tap the chat icon at the bottom of the screen.

When the call is finished, changes made by your clinician display on the exit screen.

Troubleshoot

Problem	Resolution
You have trouble connecting to the app	<ol style="list-style-type: none">1. Restart your sound processor.2. Restart the app.3. Restart the device running the app.
You don't receive notifications	Check that the app is running on your device.

General information

Labelling symbols

These symbols may appear in the Nucleus Smart App:



Manufacturer



CE registration mark with notified body number



Authorised representative in the European Community



Catalogue number



Medical Device



Unique Device Identification

Legal statement

The statements made in this guide are believed to be true and correct as of the date of publication. However, specifications are subject to change without notice.

© Cochlear Limited 2022

Trademark legal statement

ACE, Advance Off-Stylet, AOS, Ardium, AutoNRT, Autosensitivity, Baha, Baha SoftWear, BCDrive, Beam, Bring Back the Beat, Button, Carina, Cochlear, 科利耳, コクレア, 코클리어, Cochlear SoftWear, Contour, コントウア, Contour Advance, Custom Sound, DermaLock, Freedom, Hear now. And always, Hugfit, Human Design, Hybrid, Invisible Hearing, Kansa, LowPro, MET, MP3000, myCochlear, mySmartSound, NRT, Nucleus, Osia, Outcome Focused Fitting, Off-Stylet, Piezo Power, Profile, Slimline, SmartSound, Softip, SoundArc, True Wireless, the elliptical logo, Vistafix, Whisper, WindShield and Xidium are either trademarks or registered trademarks of the Cochlear group of companies.

Bluetooth is a registered trademark of Bluetooth SIG. Apple, iPad, iPhone and iPod touch are trademarks of Apple Inc, registered in the U.S. and other countries. Android is a trademark of Google Inc. Google Play and the Google Play logo are trademarks of Google LLC.

Hear now. And always

 **Cochlear Ltd** (ABN 96 002 618 073)
1 University Avenue, Macquarie University,
NSW 2109, Australia.
Tel: +61 2 9428 6555 Fax: +61 2 9428 6352

Cochlear Ltd (ABN 96 002 618 073) 14 Mars
Road, Lane Cove, NSW 2066, Australia
Tel: +61 2 9428 6555 Fax: +61 2 9428 6352

**[ECREP] Cochlear Deutschland GmbH &
Co. KG** Karl-Wiechert-Allee 76A, 30625
Hannover, Germany
Tel: +49 511 542 770 Fax: +49 511 542 7770

[CHREP] Cochlear AG EMEA Headquarters,
Peter Merian-Weg 4, 4052 Basel, Switzerland
Tel: +41 61 205 8204 Fax: +41 61 205 8205

Cochlear Americas 10350 Park Meadows
Drive, Lone Tree, CO 80124, USA
Tel: +1 303 790 9010 Fax: +1 303 792 9025

Cochlear Canada Inc 2500-120 Adelaide
Street West, Toronto, ON M5H 1T1, Canada
Tel: +1 416 972 5082 Fax: +1 416 972 5083

Cochlear Europe Ltd 6 Dashwood Lang
Road, Bourne Business Park, Addlestone,
Surrey KT15 2HJ, United Kingdom
Tel: +44 1932 26 3400 Fax: +44 1932 26 3426

Cochlear Benelux NV Schaliënhoeverdreef
20 i, B-2800 Mechelen, Belgium
Tel: +32 15 79 55 11 Fax: +32 15 79 55 70

Cochlear France S.A.S. 135 Route de
Saint-Simon, 31035 Toulouse, France
Tel: +33 5 34 63 85 85 (International) or 0805
200 016 (National) Fax: +33 5 34 63 85 80

Cochlear Italia S.r.l. Via Trattati Comunitari
Europei 1957-2007 n.17, 40127 Bologna
(BO), Italy
Tel: +39 051 601 53 11 Fax: +39 051 39 20 62

Cochlear Nordic AB Konstruktionsvägen 14,
435 33 Mölnlycke, Sweden
Tel: +46 31 335 14 61 Fax: +46 31 335 14 60

www.cochlear.com



**Cochlear Tıbbi Cihazlar ve Sağlık
Hizmetleri Ltd. Şti.** Çubuklu Mah. Boğaziçi
Cad., Boğaziçi Plaza No: 6/1, Kavacık,
TR-34805 Beykoz-Istanbul, Turkey
Tel: +90 216 538 5900 Fax: +90 216 538 5919

Cochlear (HK) Limited Room 1404-1406,
14/F, Leighton Centre, 77 Leighton Road,
Causeway Bay, Hong Kong
Tel: +852 2530 5773 Fax: +852 2530 5183

Cochlear Korea Ltd 2nd Floor, Yongsan
Centreville Asterium, 25, Hangang-daero
30 gil, Yongsan-gu, Seoul, Korea (04386)
Tel: +82 2 533 4450 Fax: +82 2 533 8408

Cochlear Medical Device (Beijing) Co., Ltd
Unit 2608-2617, 26th Floor, No.9 Building,
No.91 Jianguo Road, Chaoyang District,
Beijing 100022, P.R. China
Tel: +86 10 5909 7800 Fax: +86 10 5909 7900

**Cochlear Medical Device Company India
Pvt. Ltd** Ground Floor, Platina Building, Plot
No C-59, G-Block, Bandra Kurla Complex,
Bandra (E), Mumbai - 400 051, India
Tel: +91 22 6112 1111 Fax: +91 22 6112 1100

**株式会社日本コクレア(Nihon Cochlear
Co Ltd)** 〒113-0033 東京都文京区本郷
2-3-7 お茶の水元町ビル
Tel: +81 3 3817 0241 Fax: +81 3 3817 0245

Cochlear Middle East FZ-LLC Dubai
Healthcare City, Al Razi Building 64, Block A,
Ground Floor, Offices IR1 and IR2, Dubai,
United Arab Emirates
Tel: +971 4 818 4400 Fax: +971 4 361 8925

Cochlear Latinoamérica S.A. International
Business Park, Building 3835, Office 403,
Panama Pacifico, Panama
Tel: +507 830 6220 Fax: +507 830 6218

Cochlear NZ Limited Level 4, Takapuna
Towers, 19-21 Como St, Takapuna, Auckland
0622, New Zealand
Tel: + 64 9 914 1983 Fax: 0800 886 036